





A R T E M & J A M E S M A G N E T I C C O N C E P T

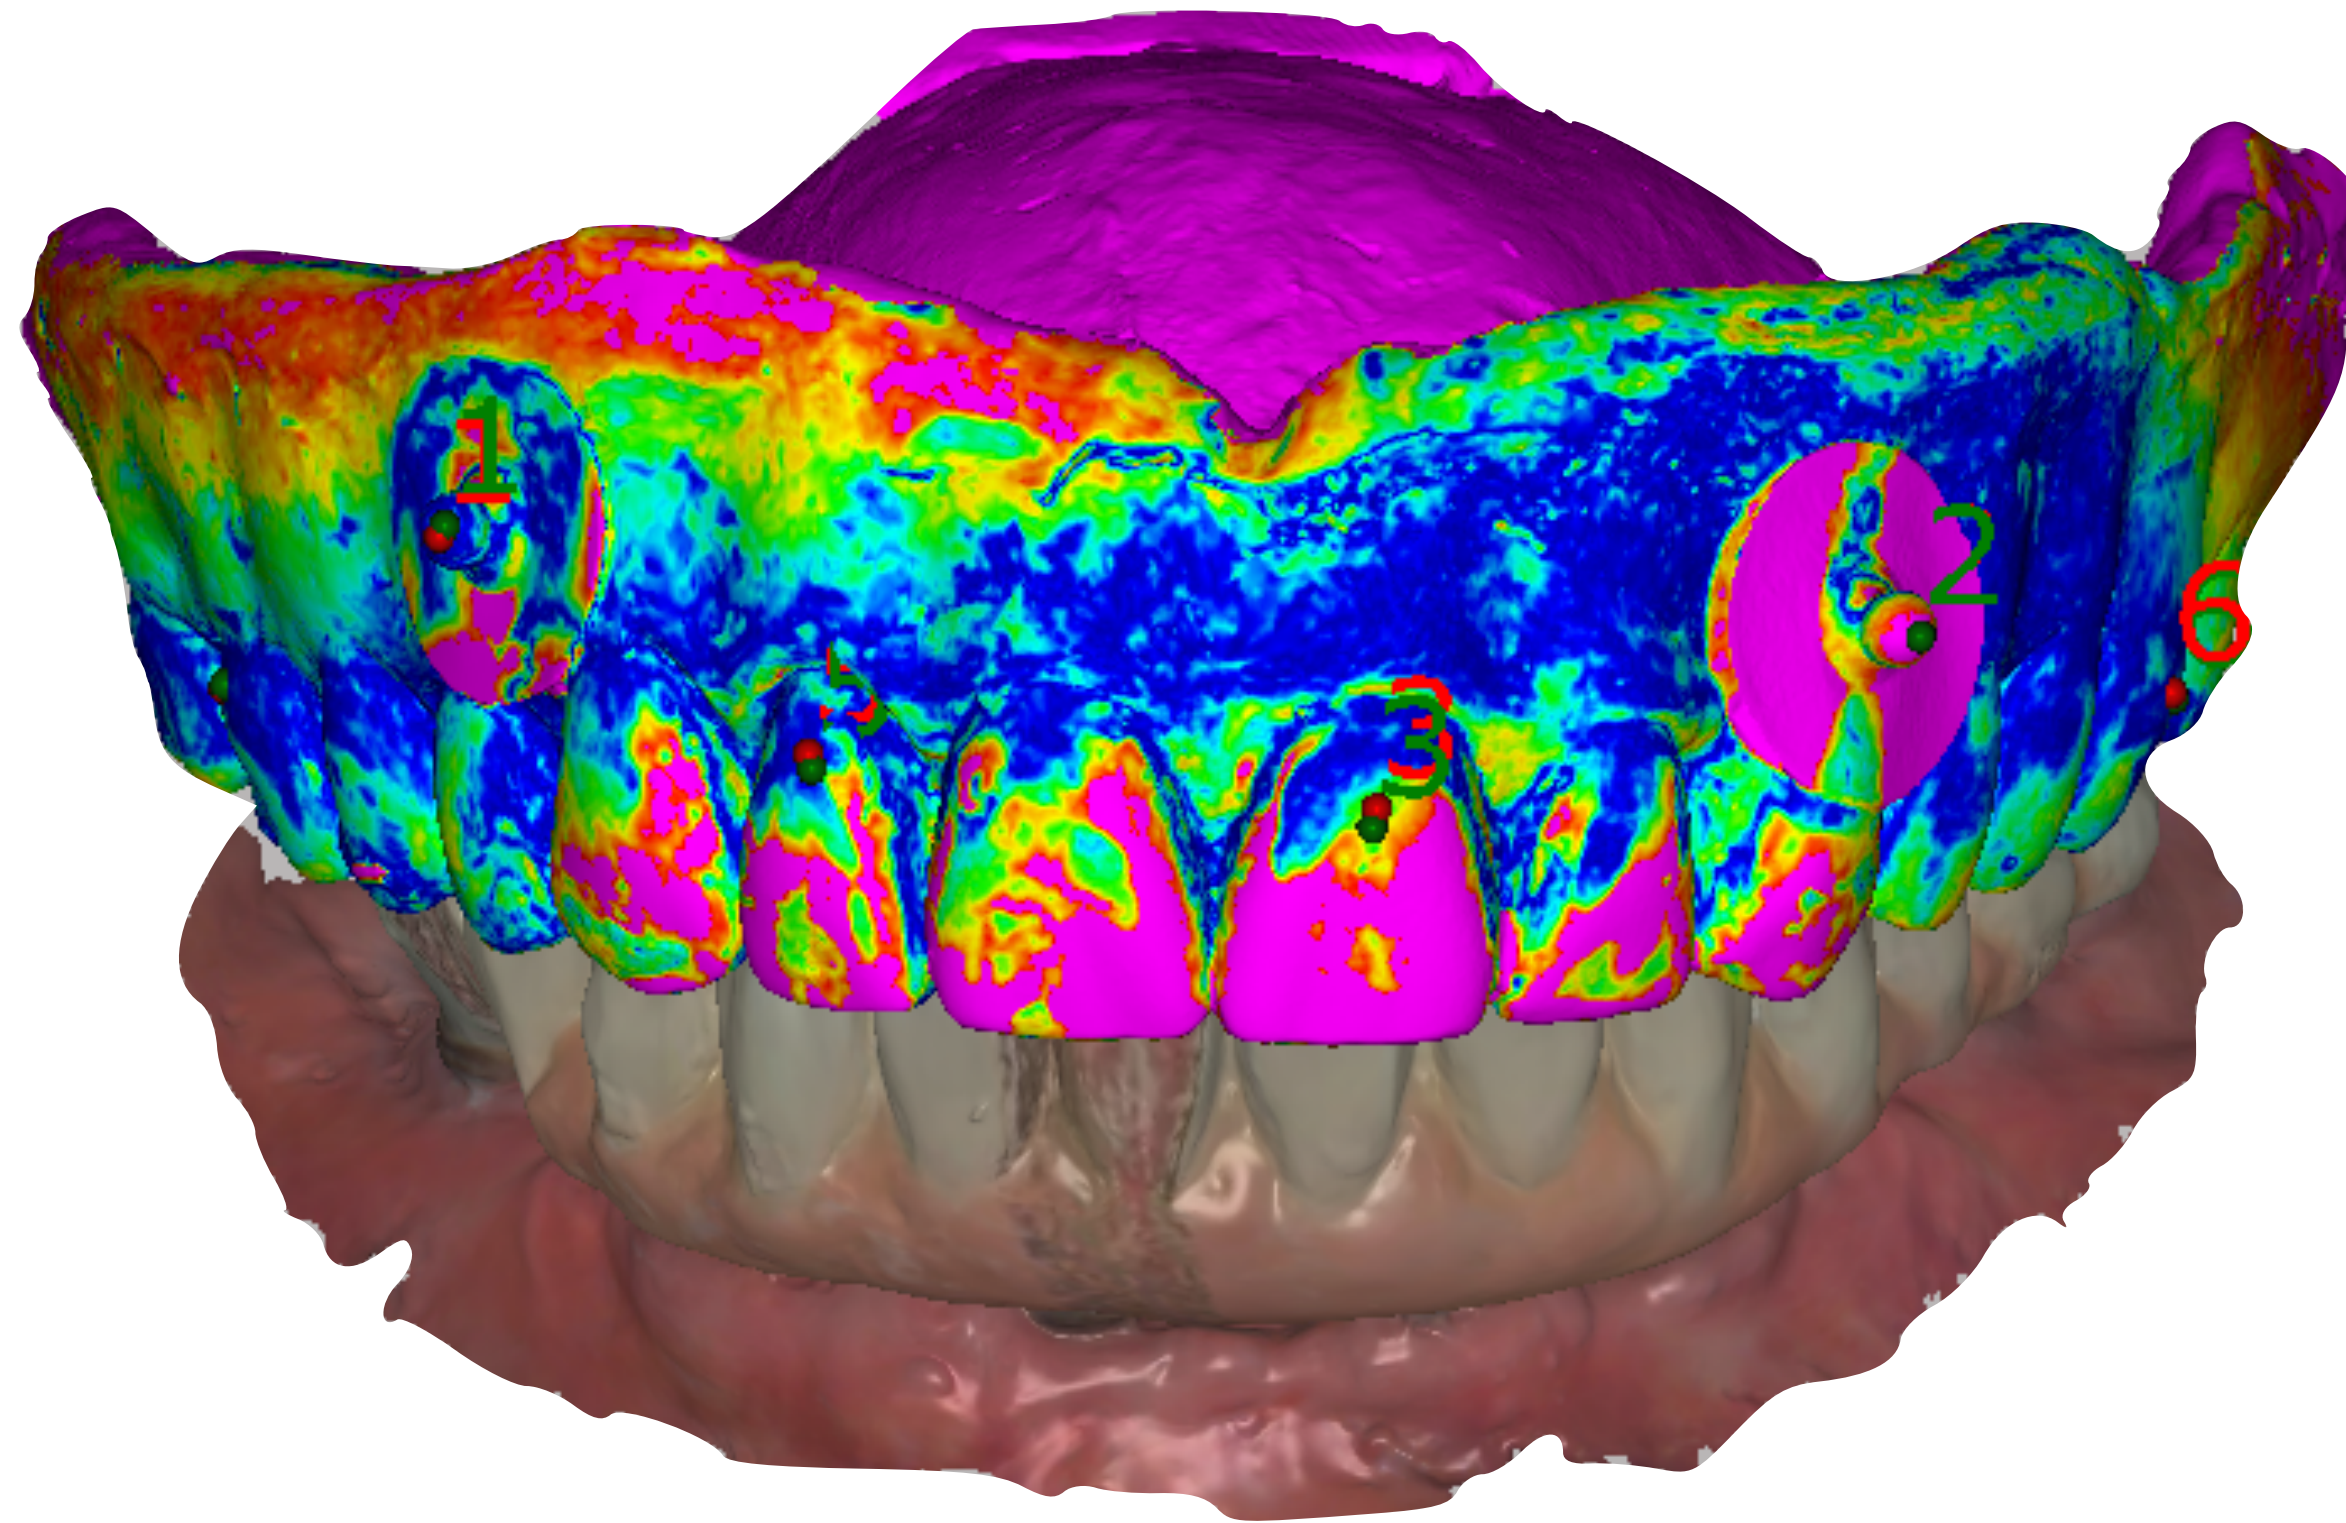


DUAL SCAN PROTOCOL

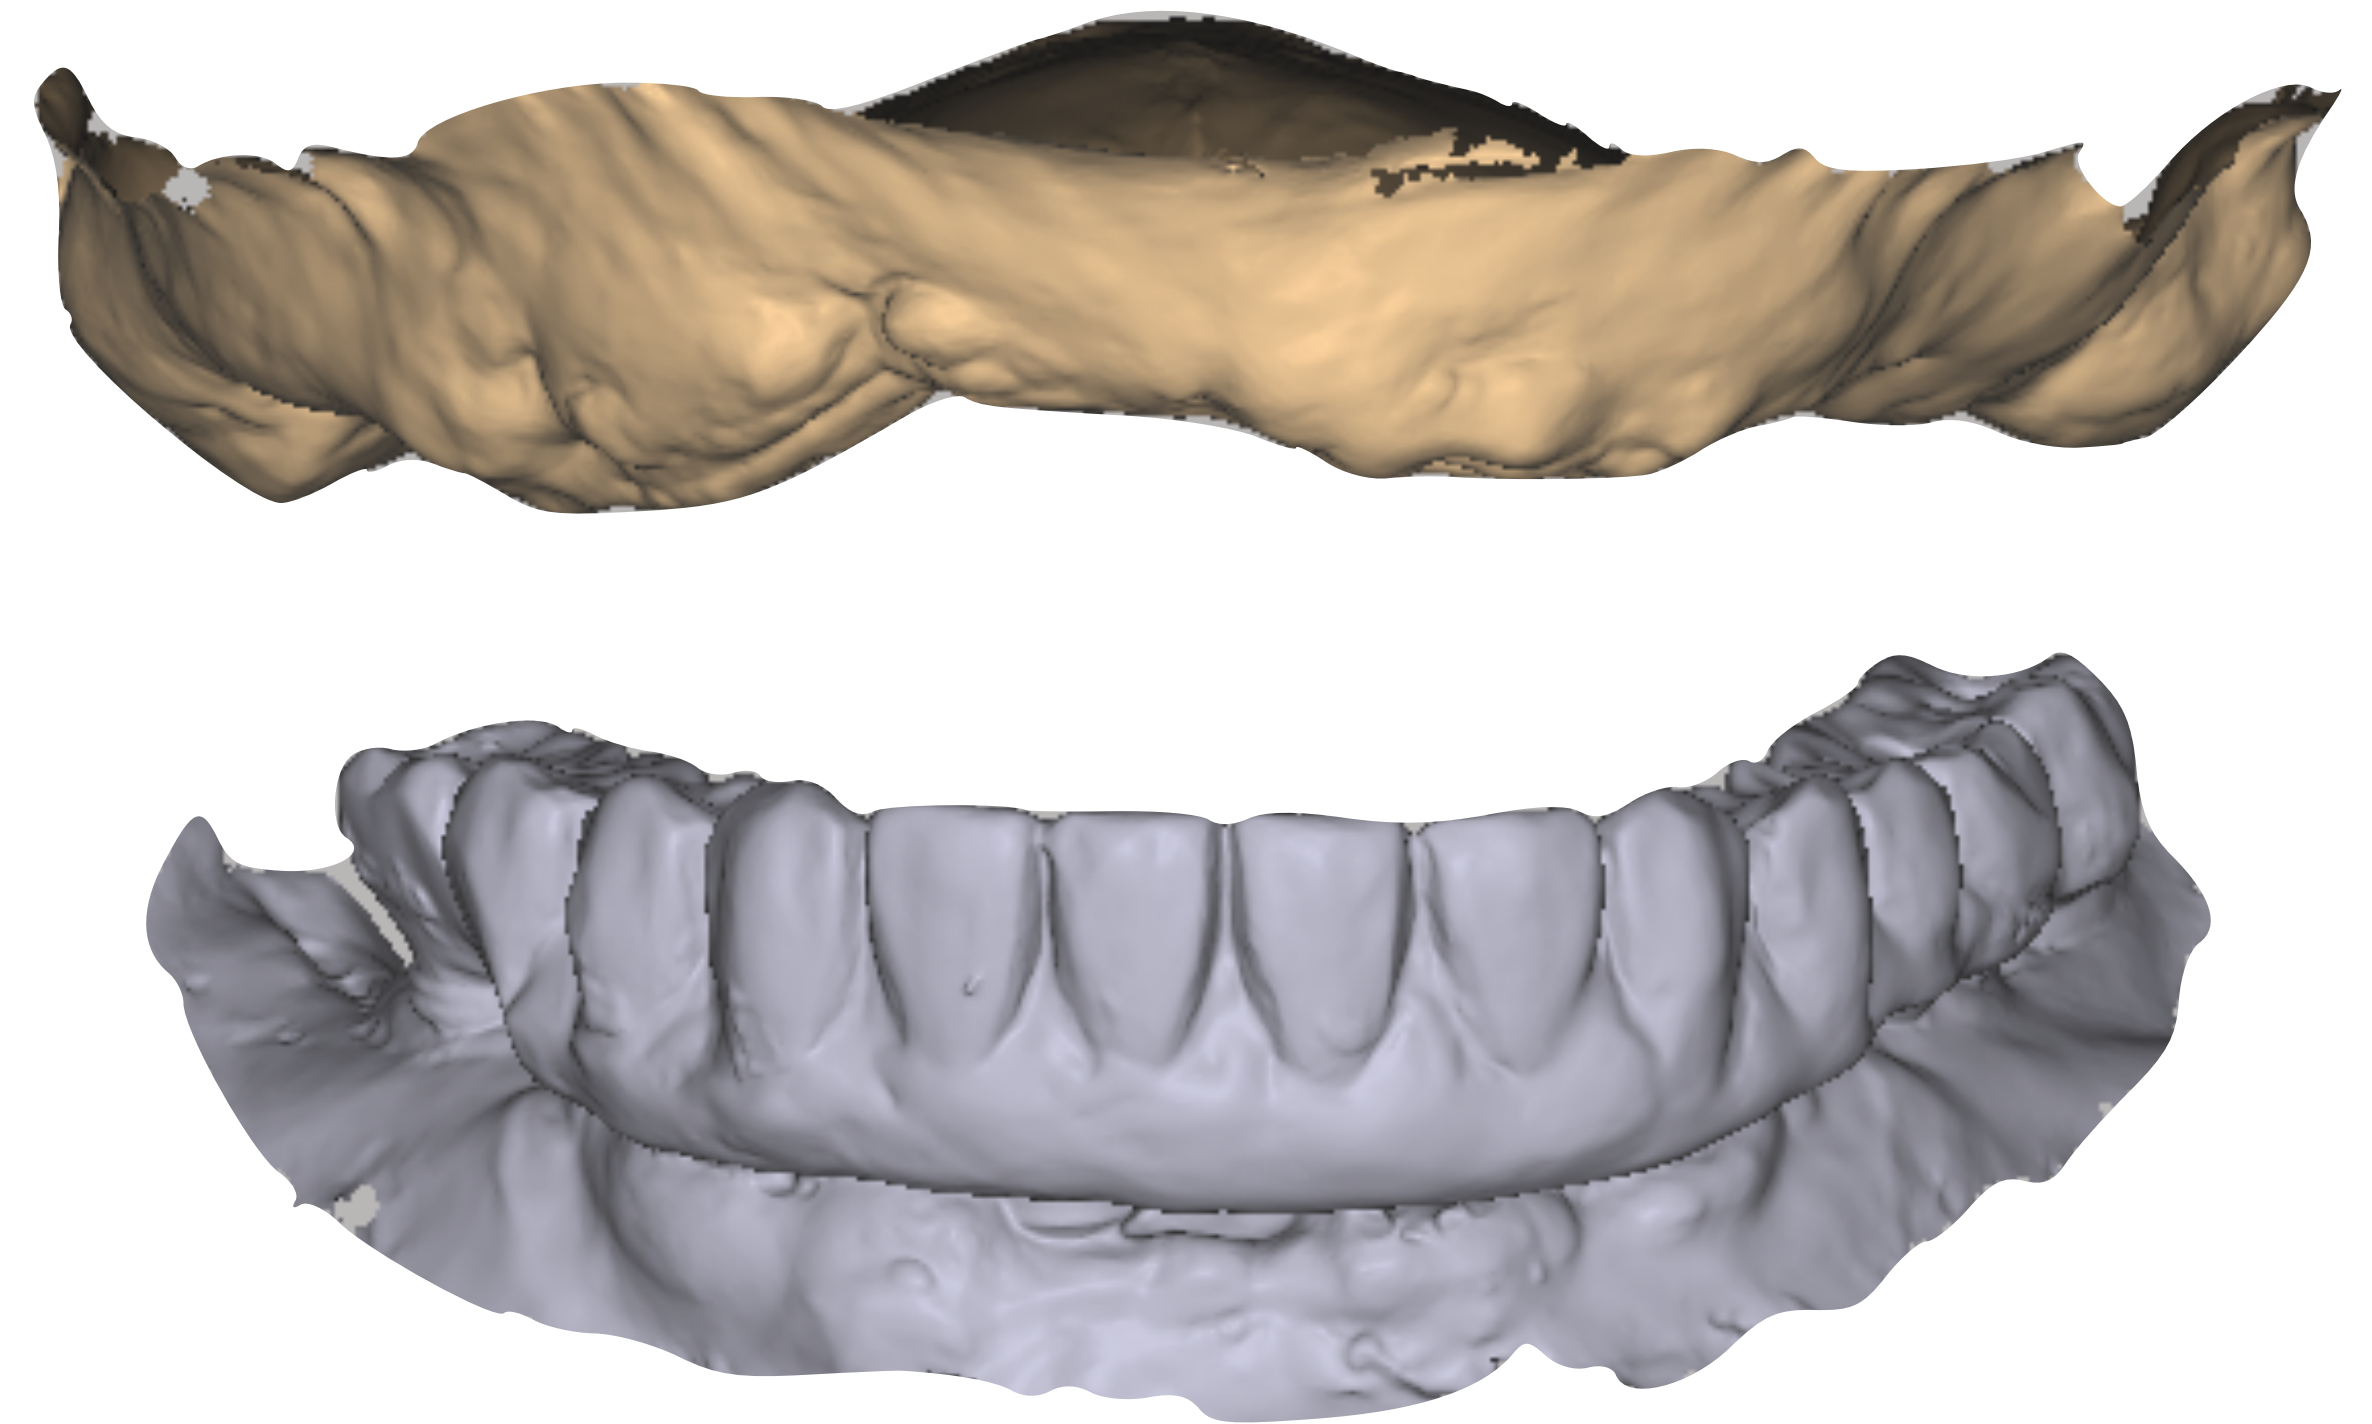



DIGITALLY STABILIZED
VERTICAL DIMENSION

DR. ALEJANDRO JAMES OROZCO

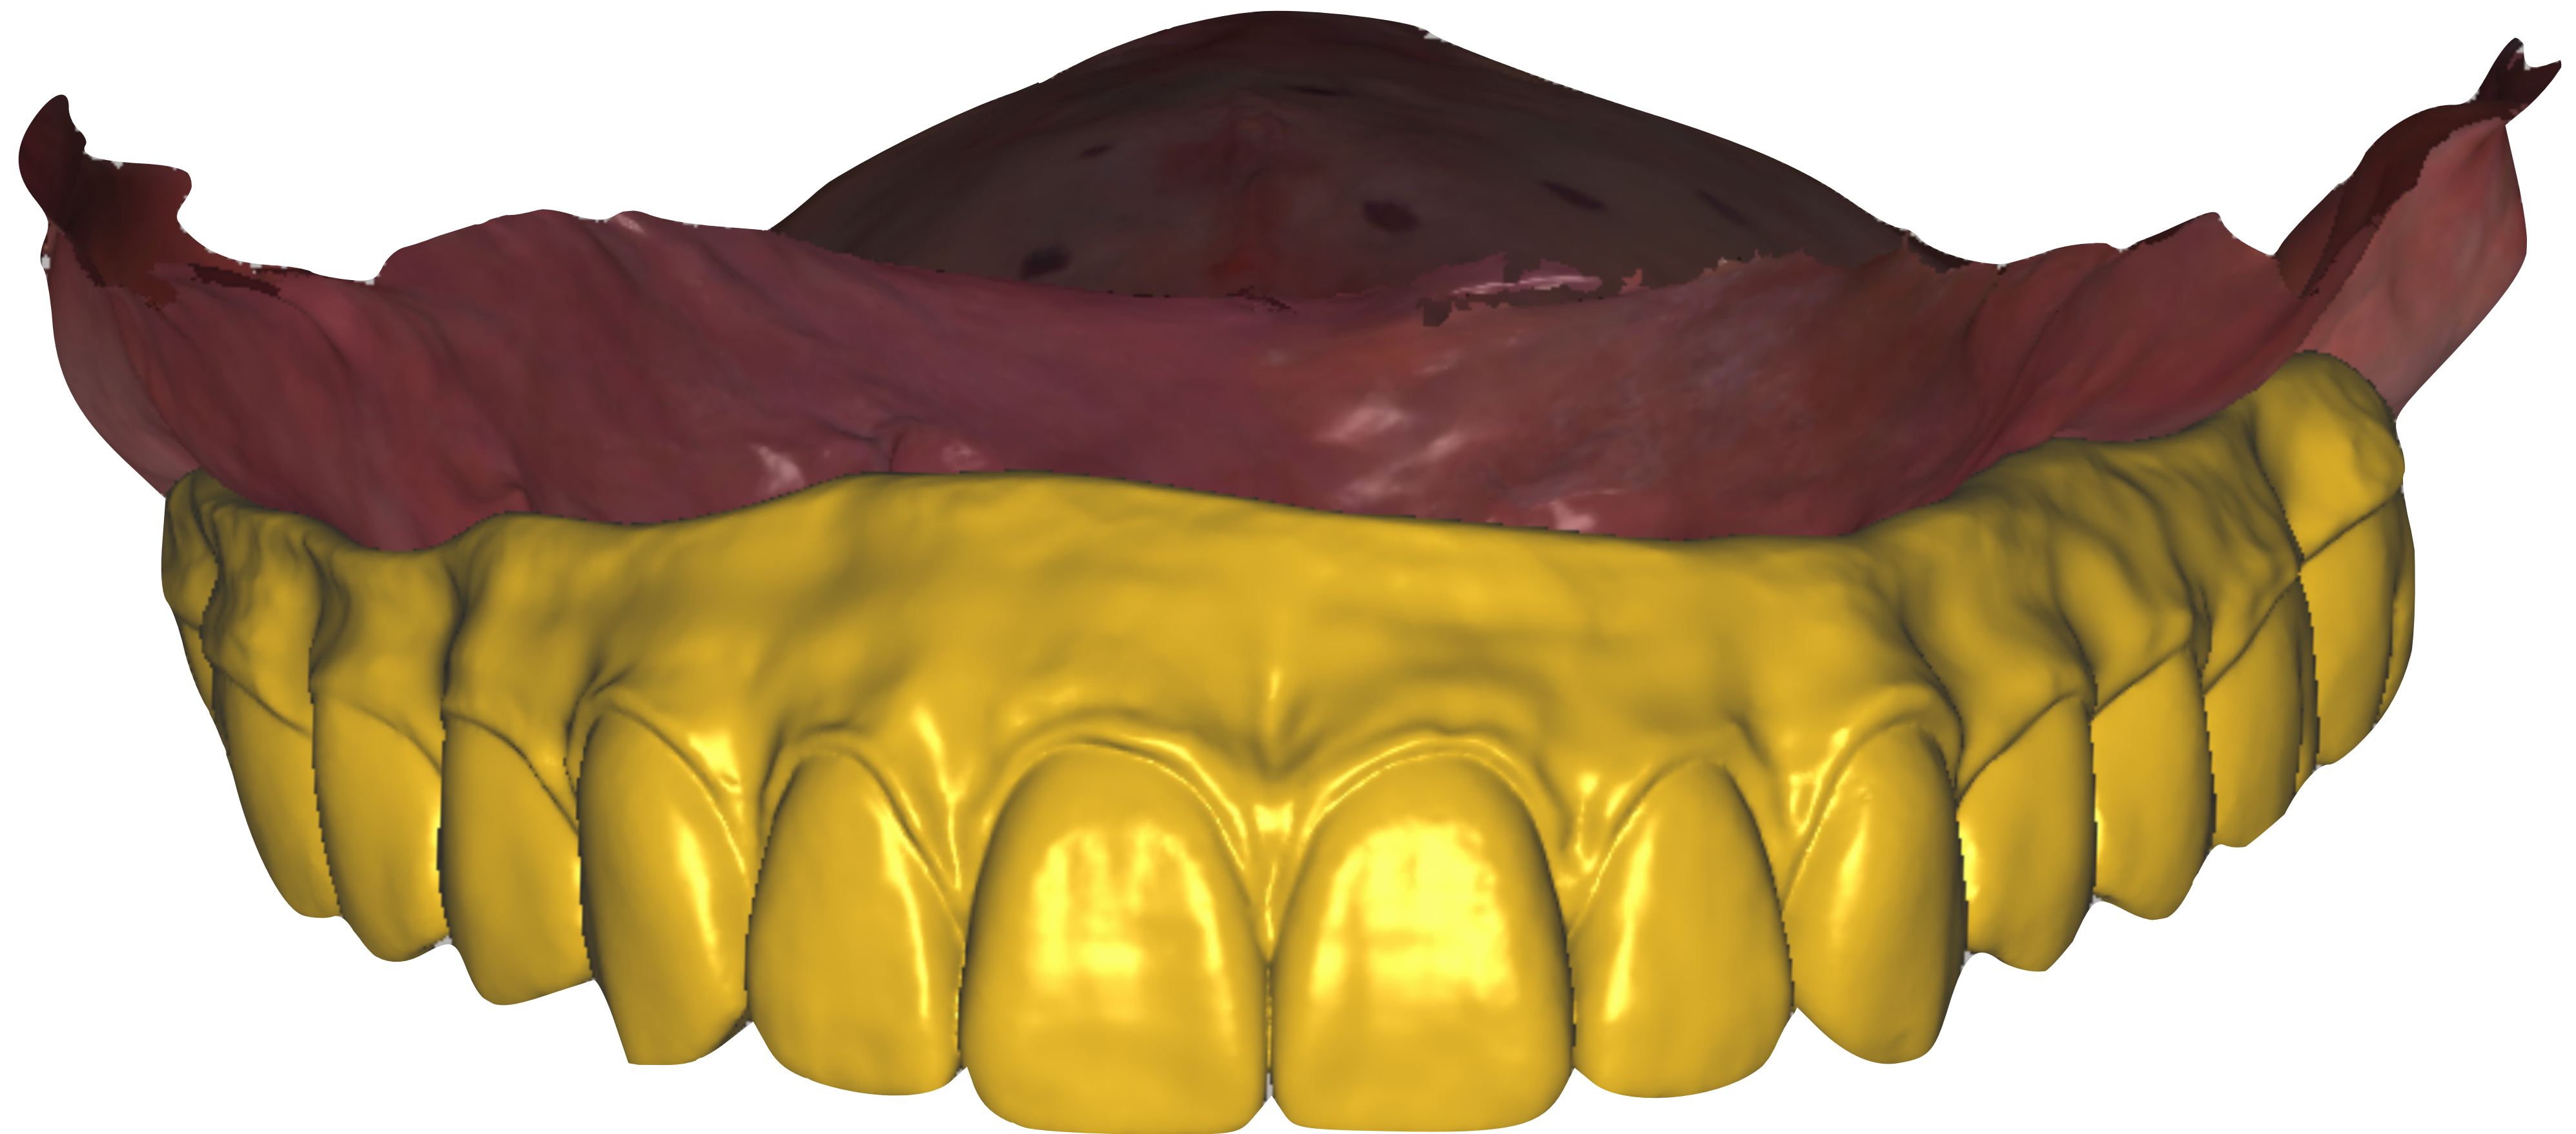

ARTMES PROVISIONAL PROTOTYPE

DR. ALEJANDRO JAMES OROZCO

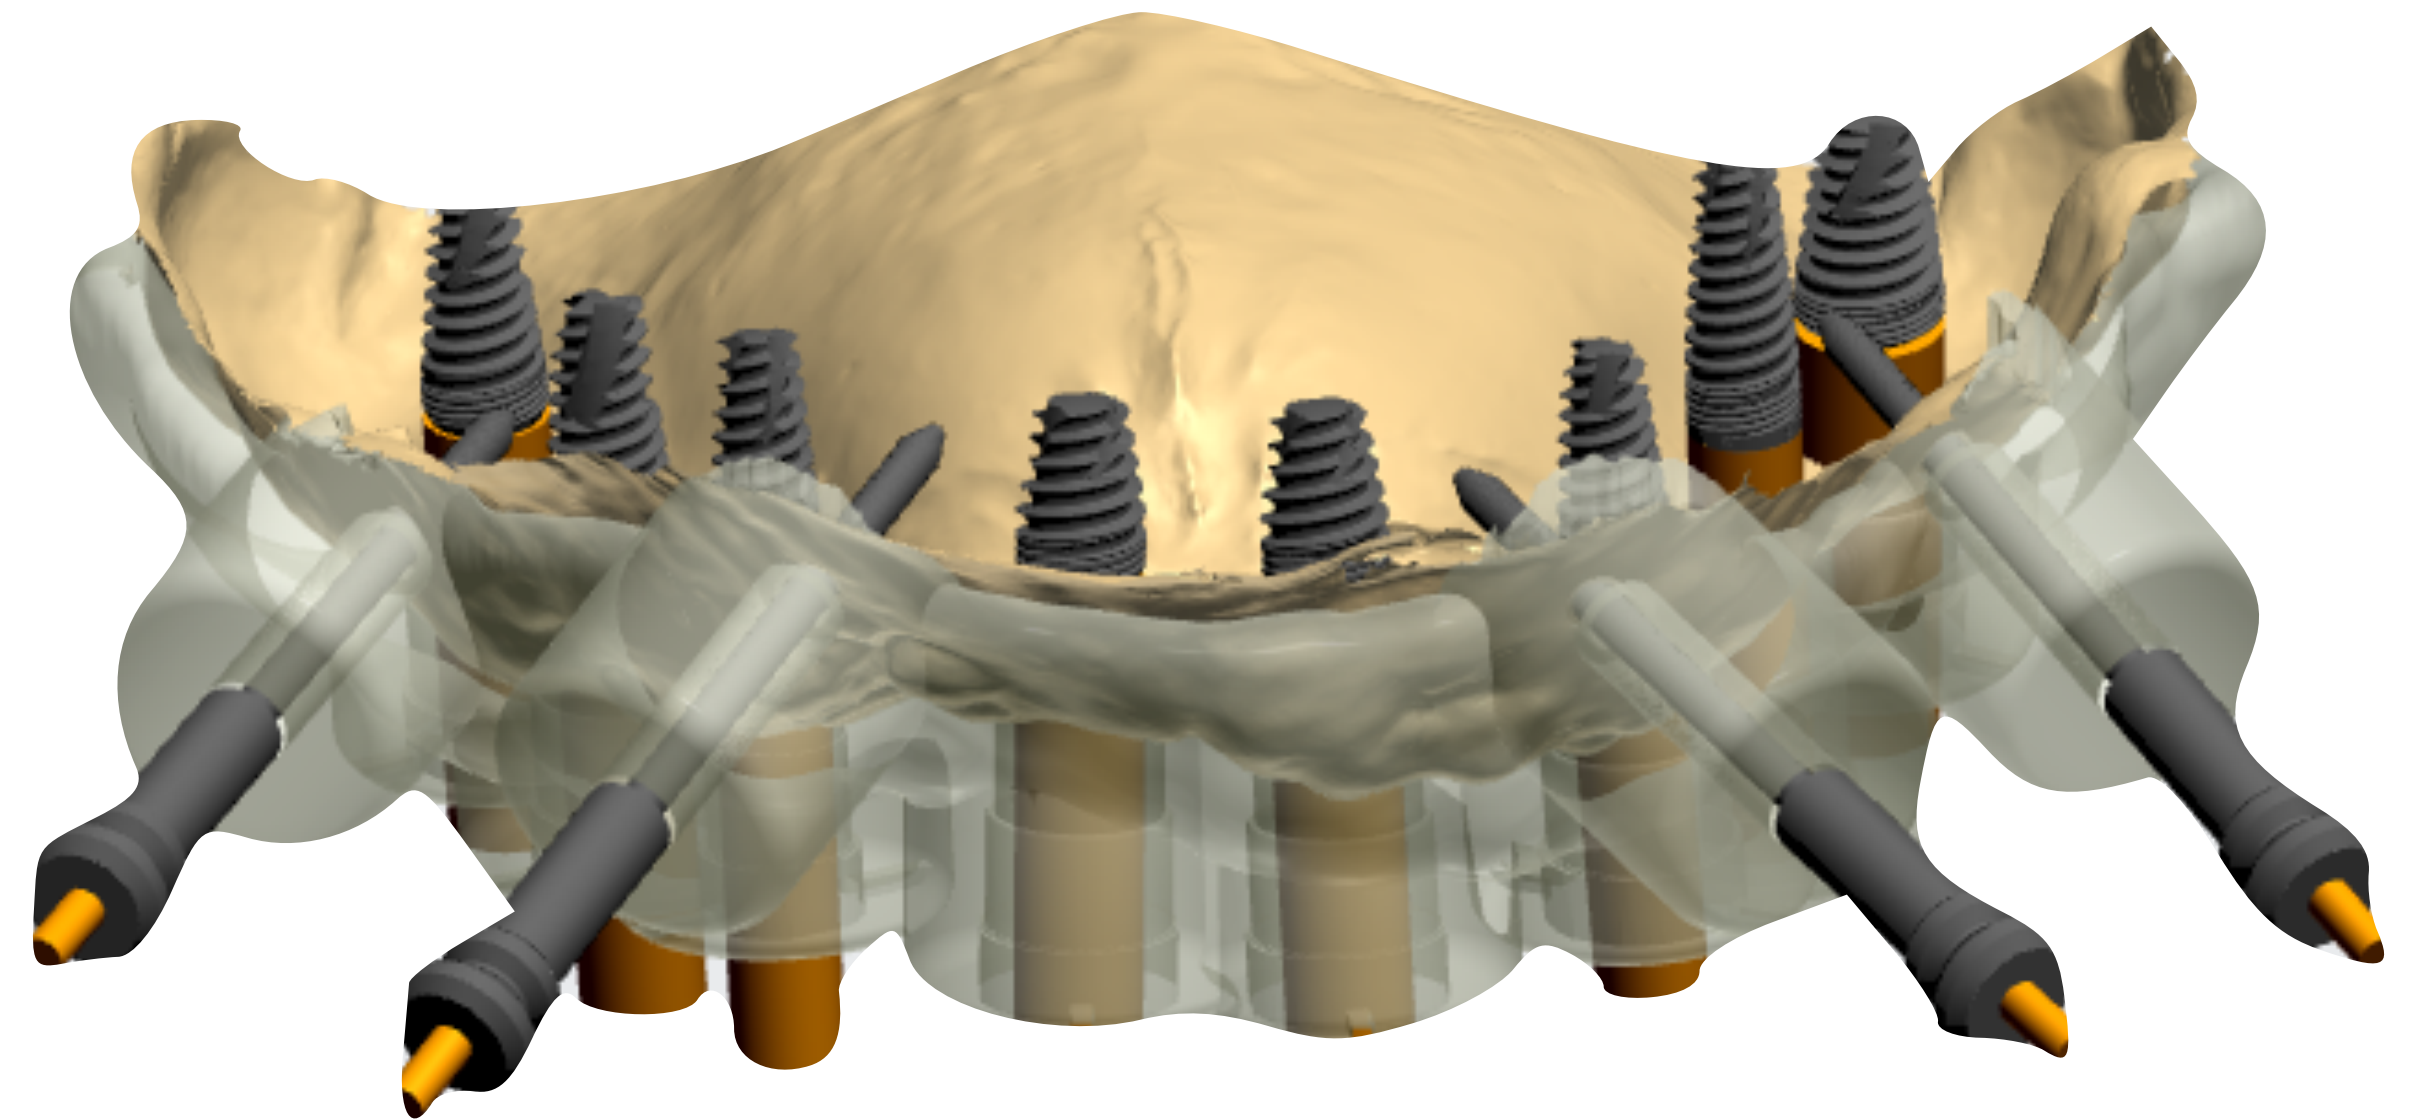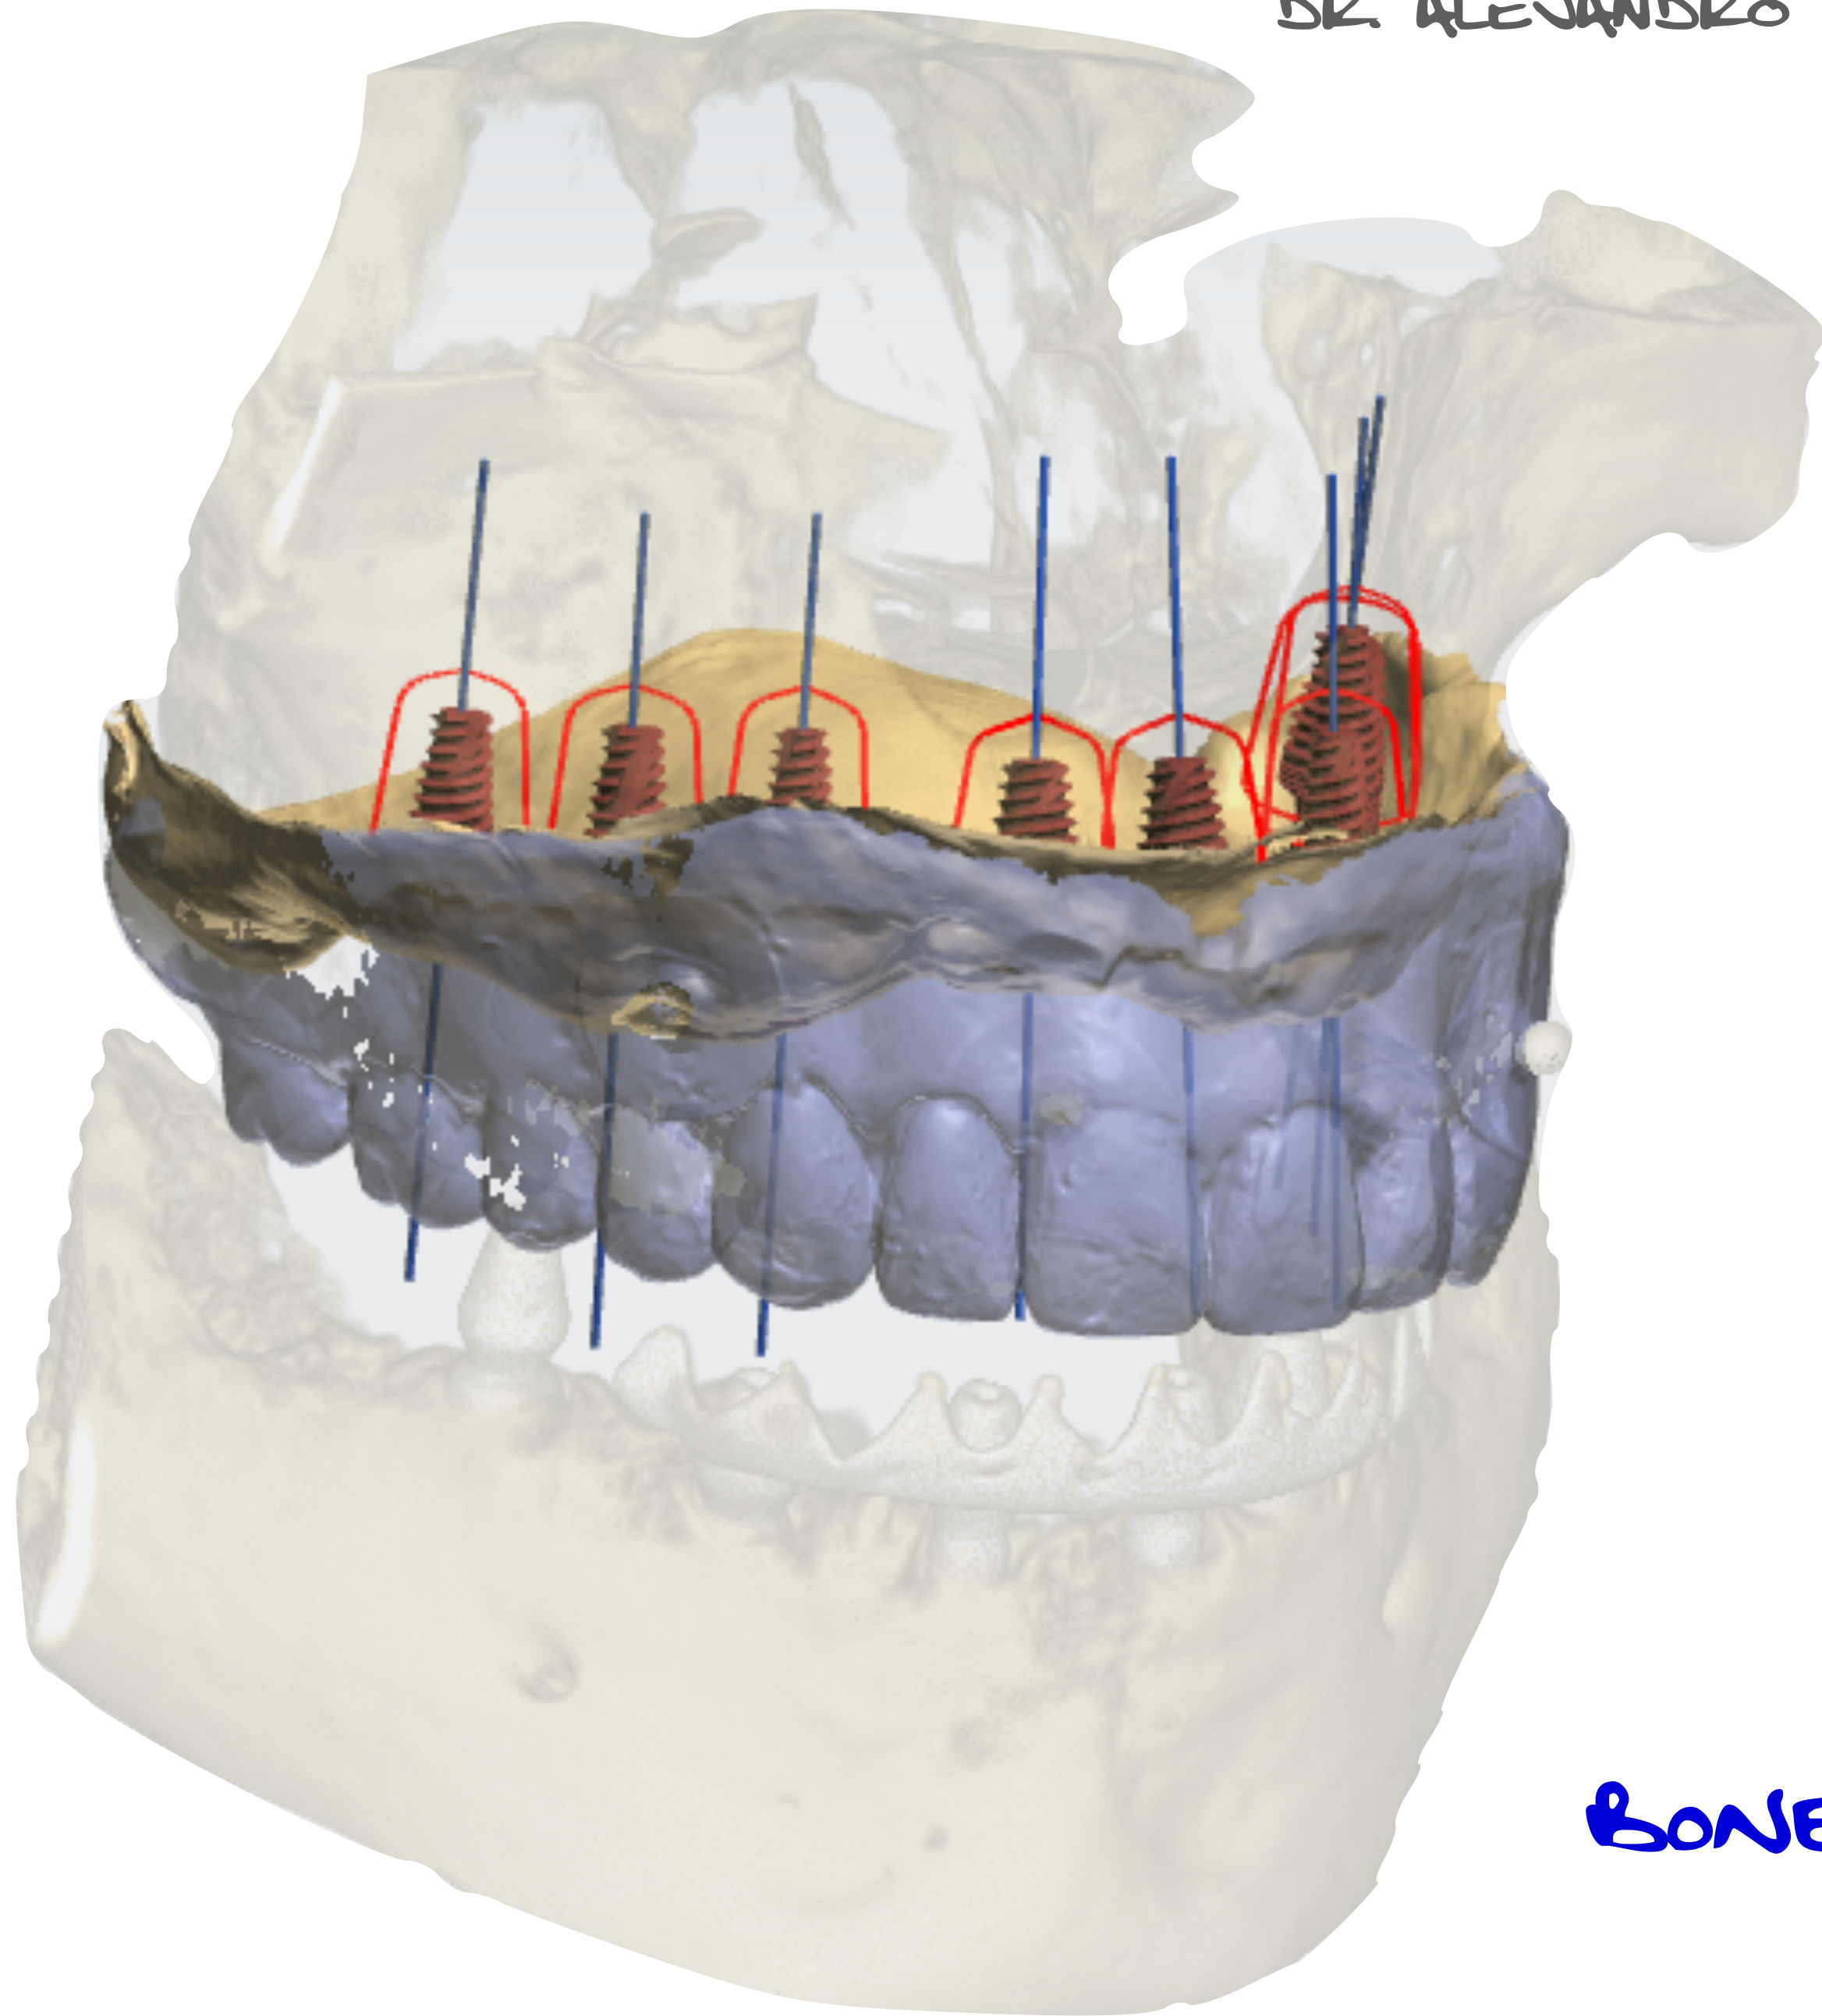

BONE A PROST ORIENTED IMPLANT PLANING

DR. ALEJANDRO JAMES OROZCO



GUIDES




TEMPS

MODELS




DR. ALEJANDRO JAMES OROZCO

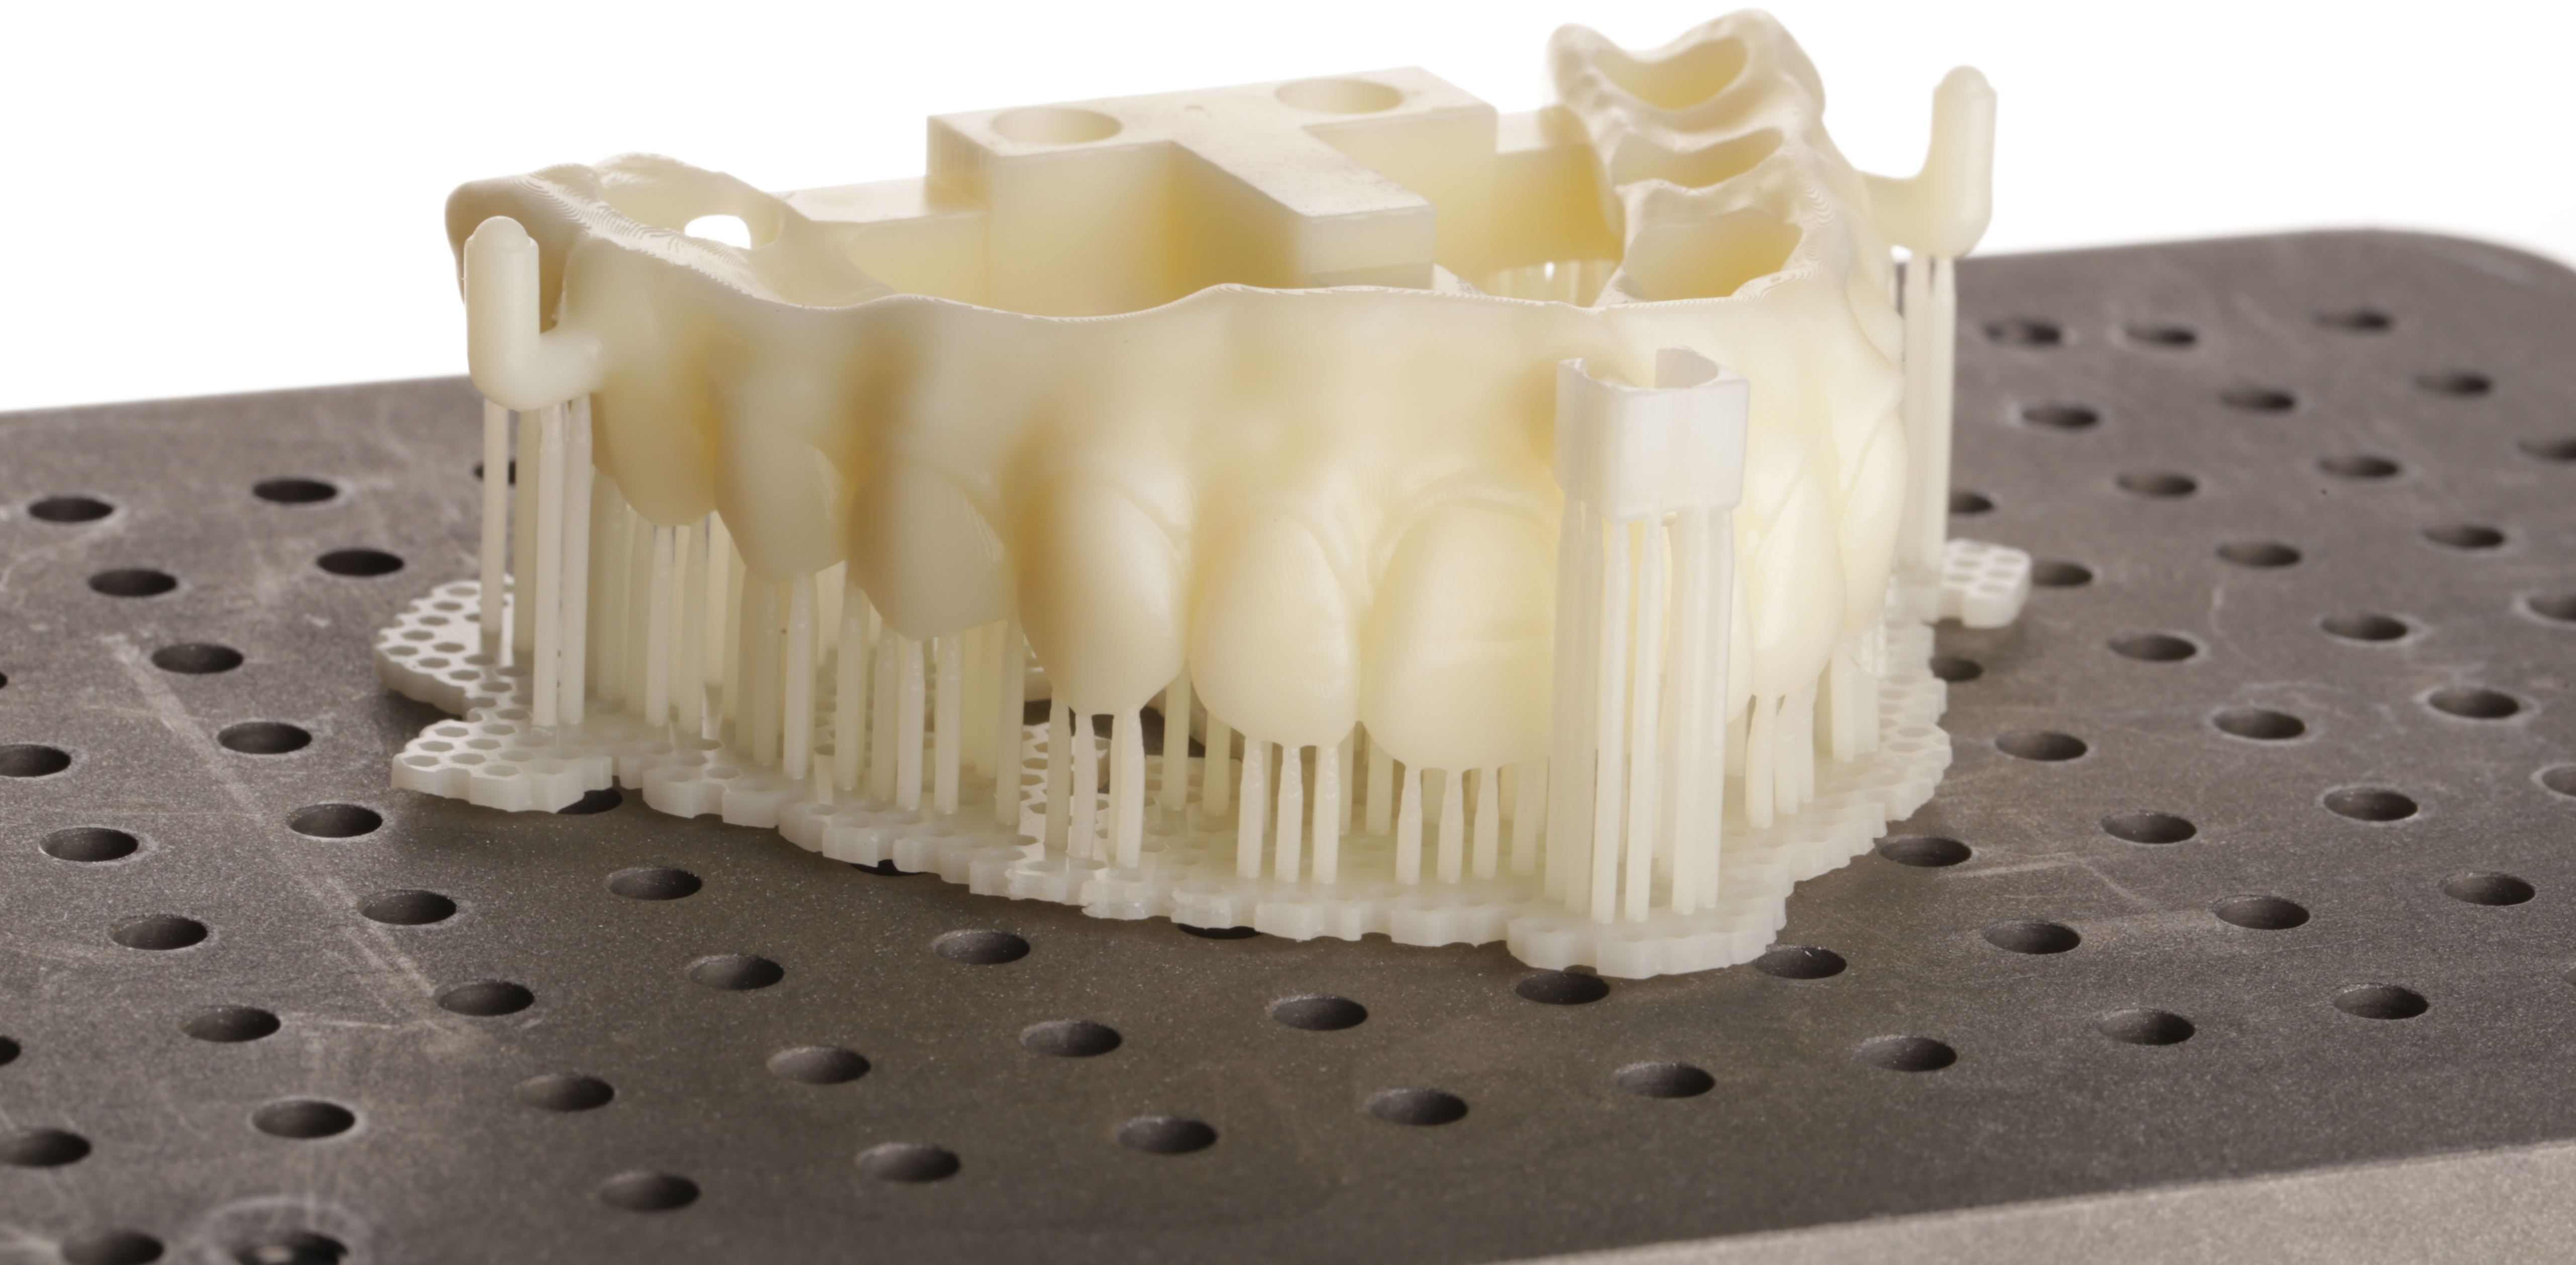


DR. ALEJANDRO JAMES OROZCO

ARTMES PRINTED PROVISIONAL

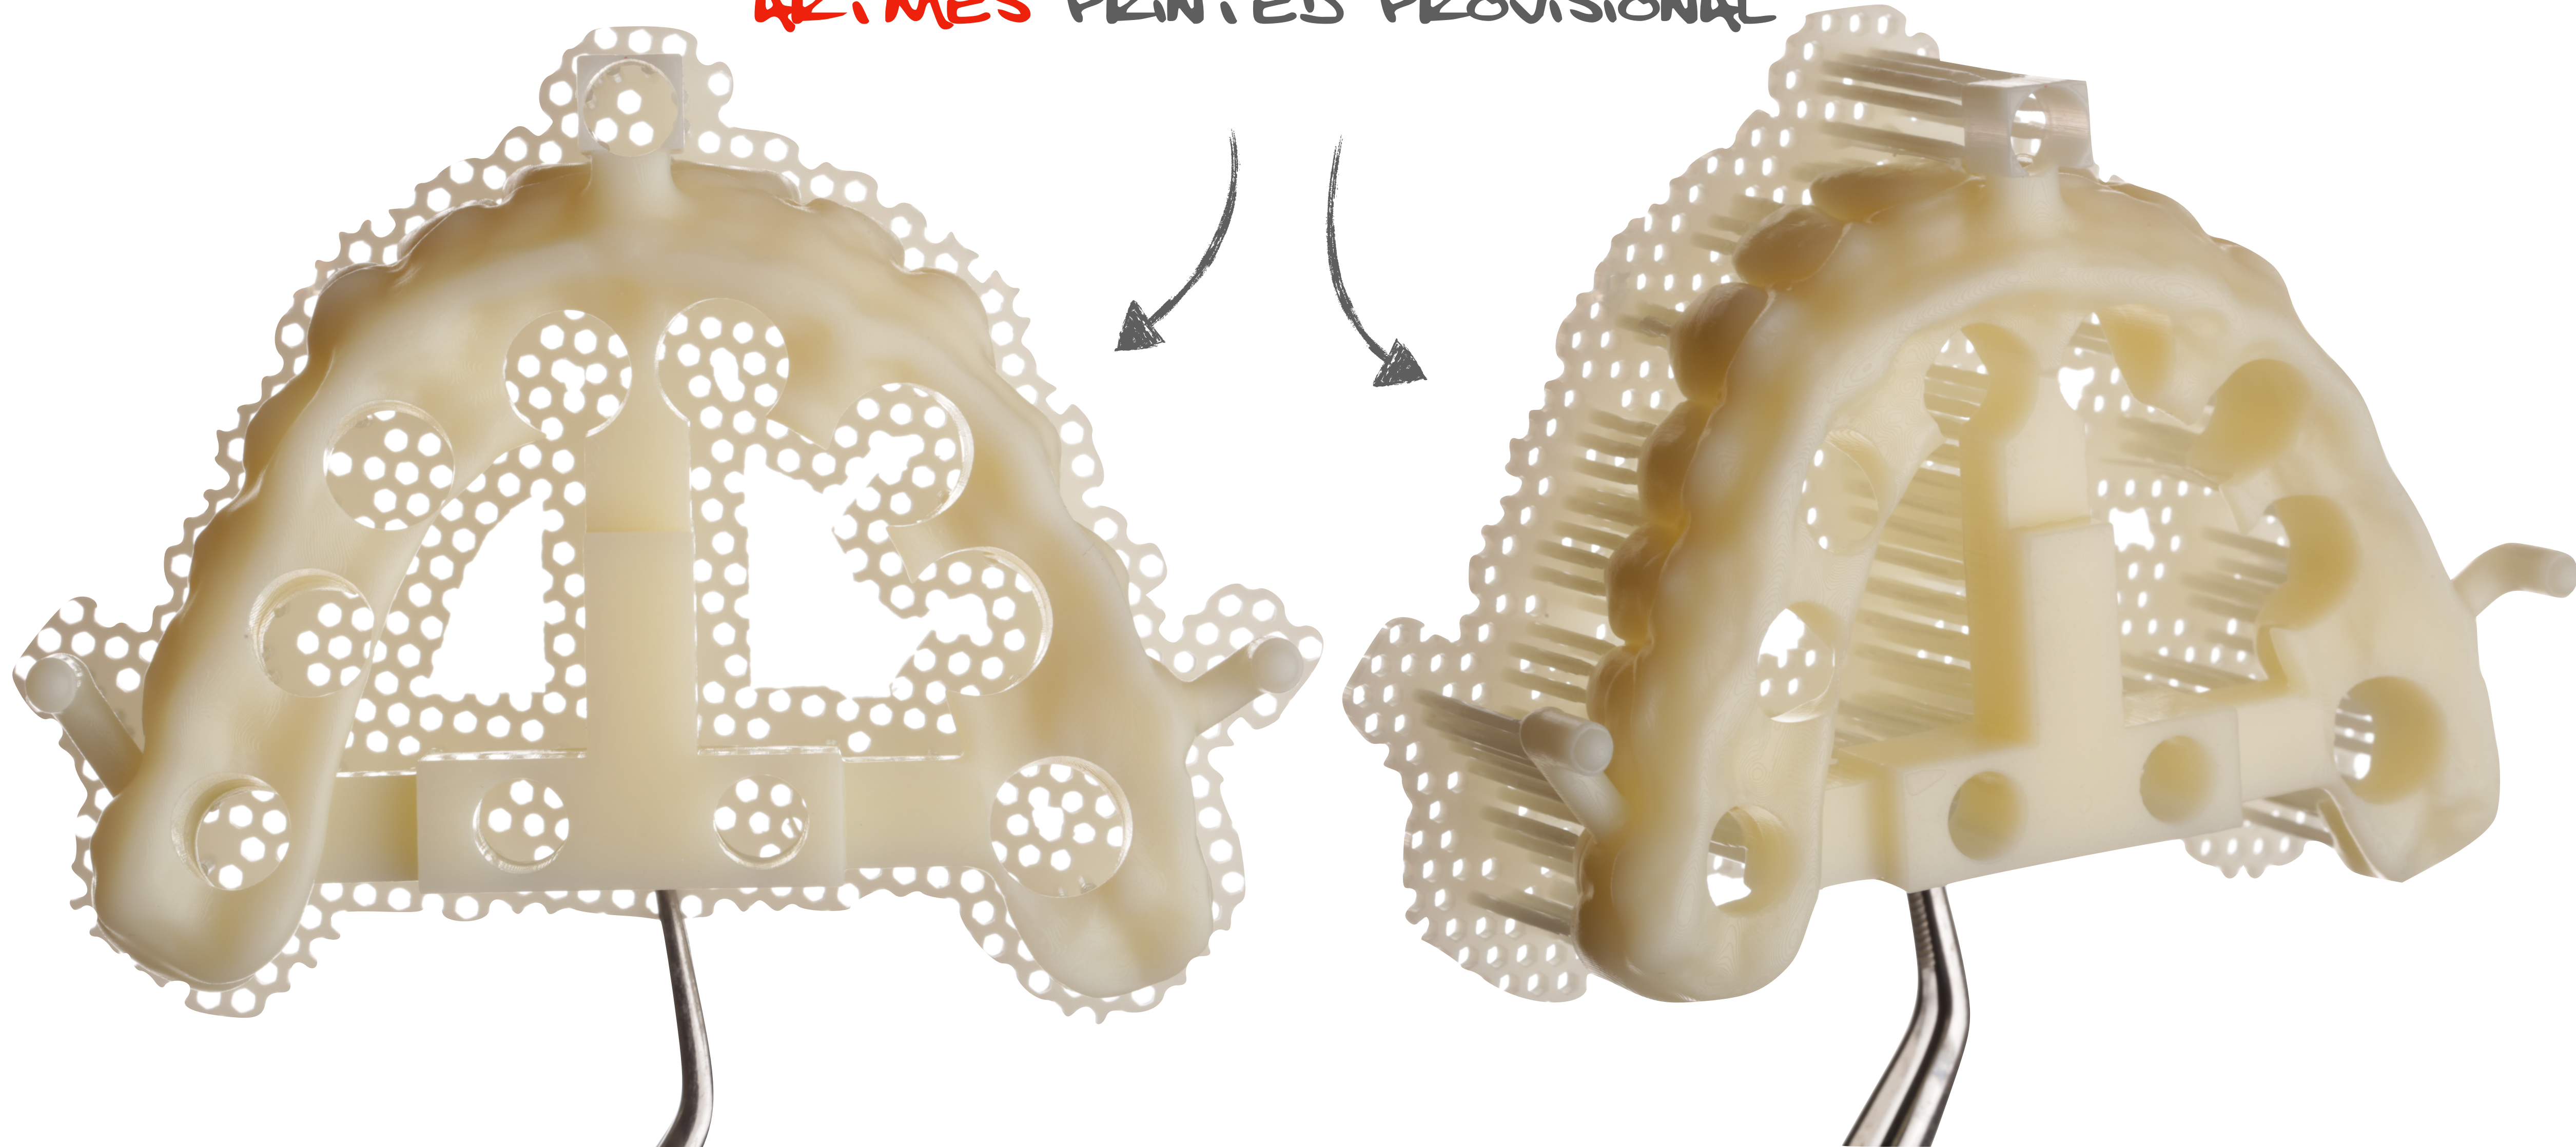

DR. ALEJANDRO JAMES OROZCO


MODEL VERIFICATION

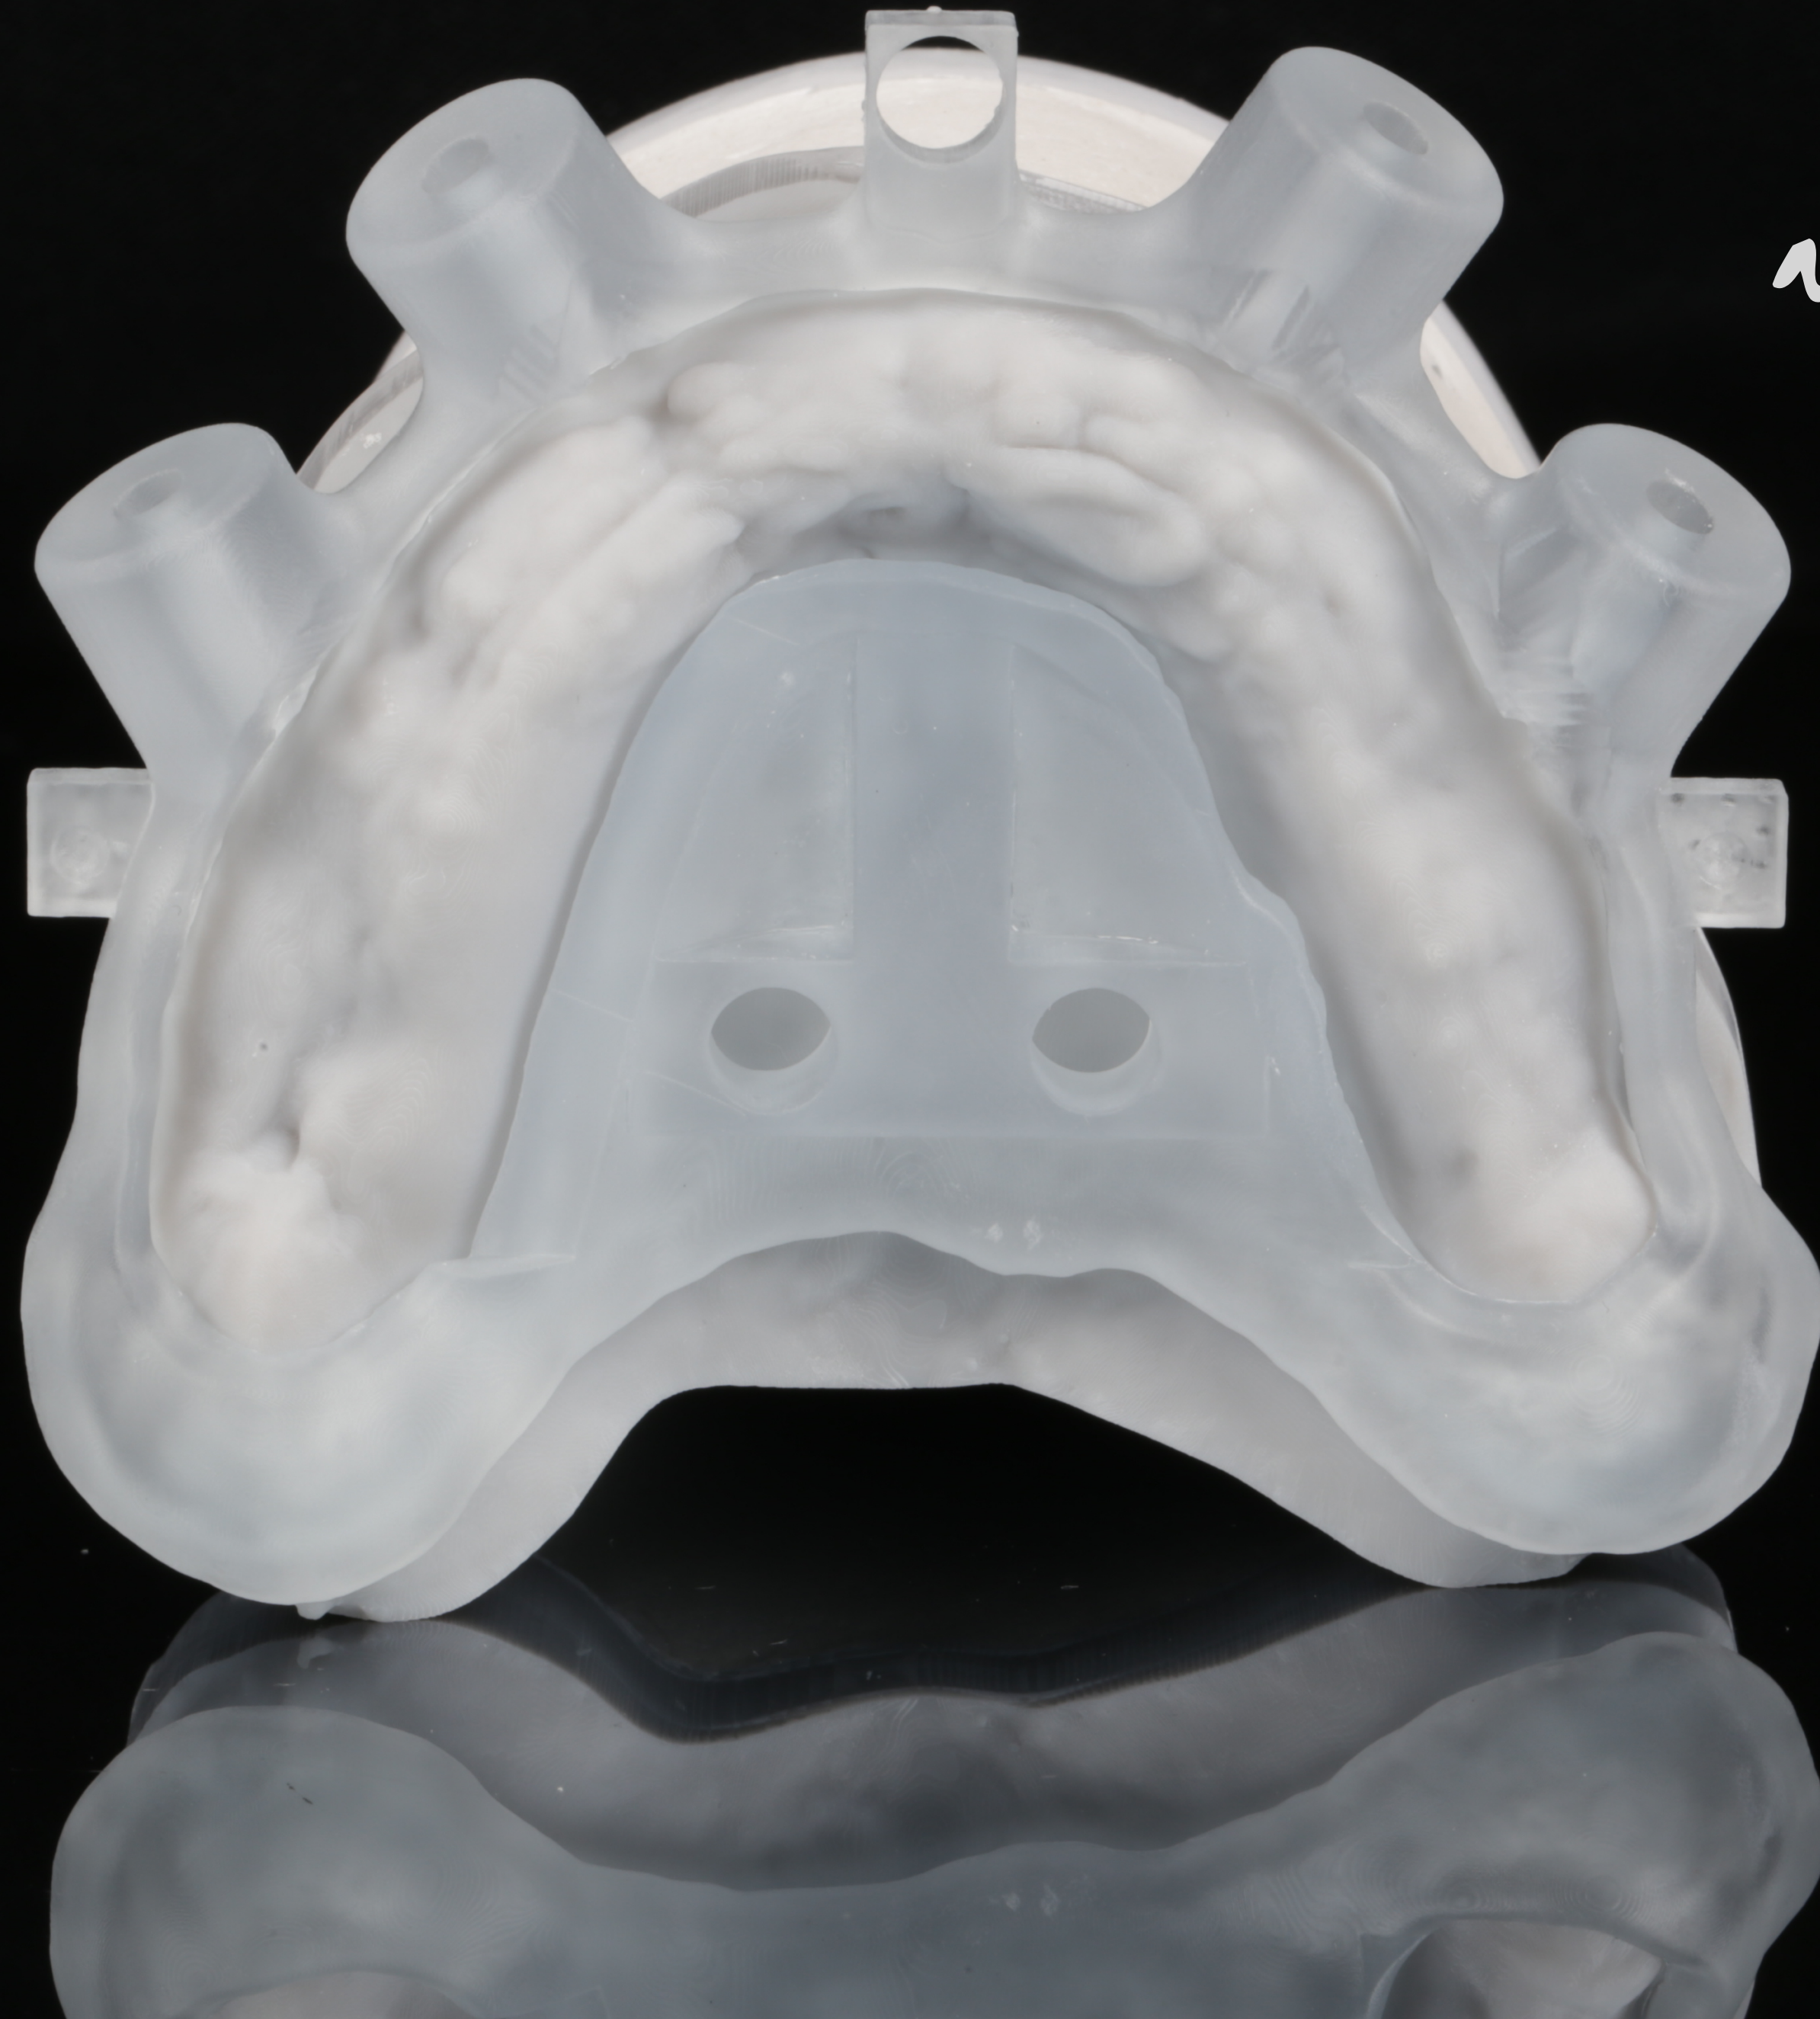

TRY-IN



FINAL PROVISIONAL

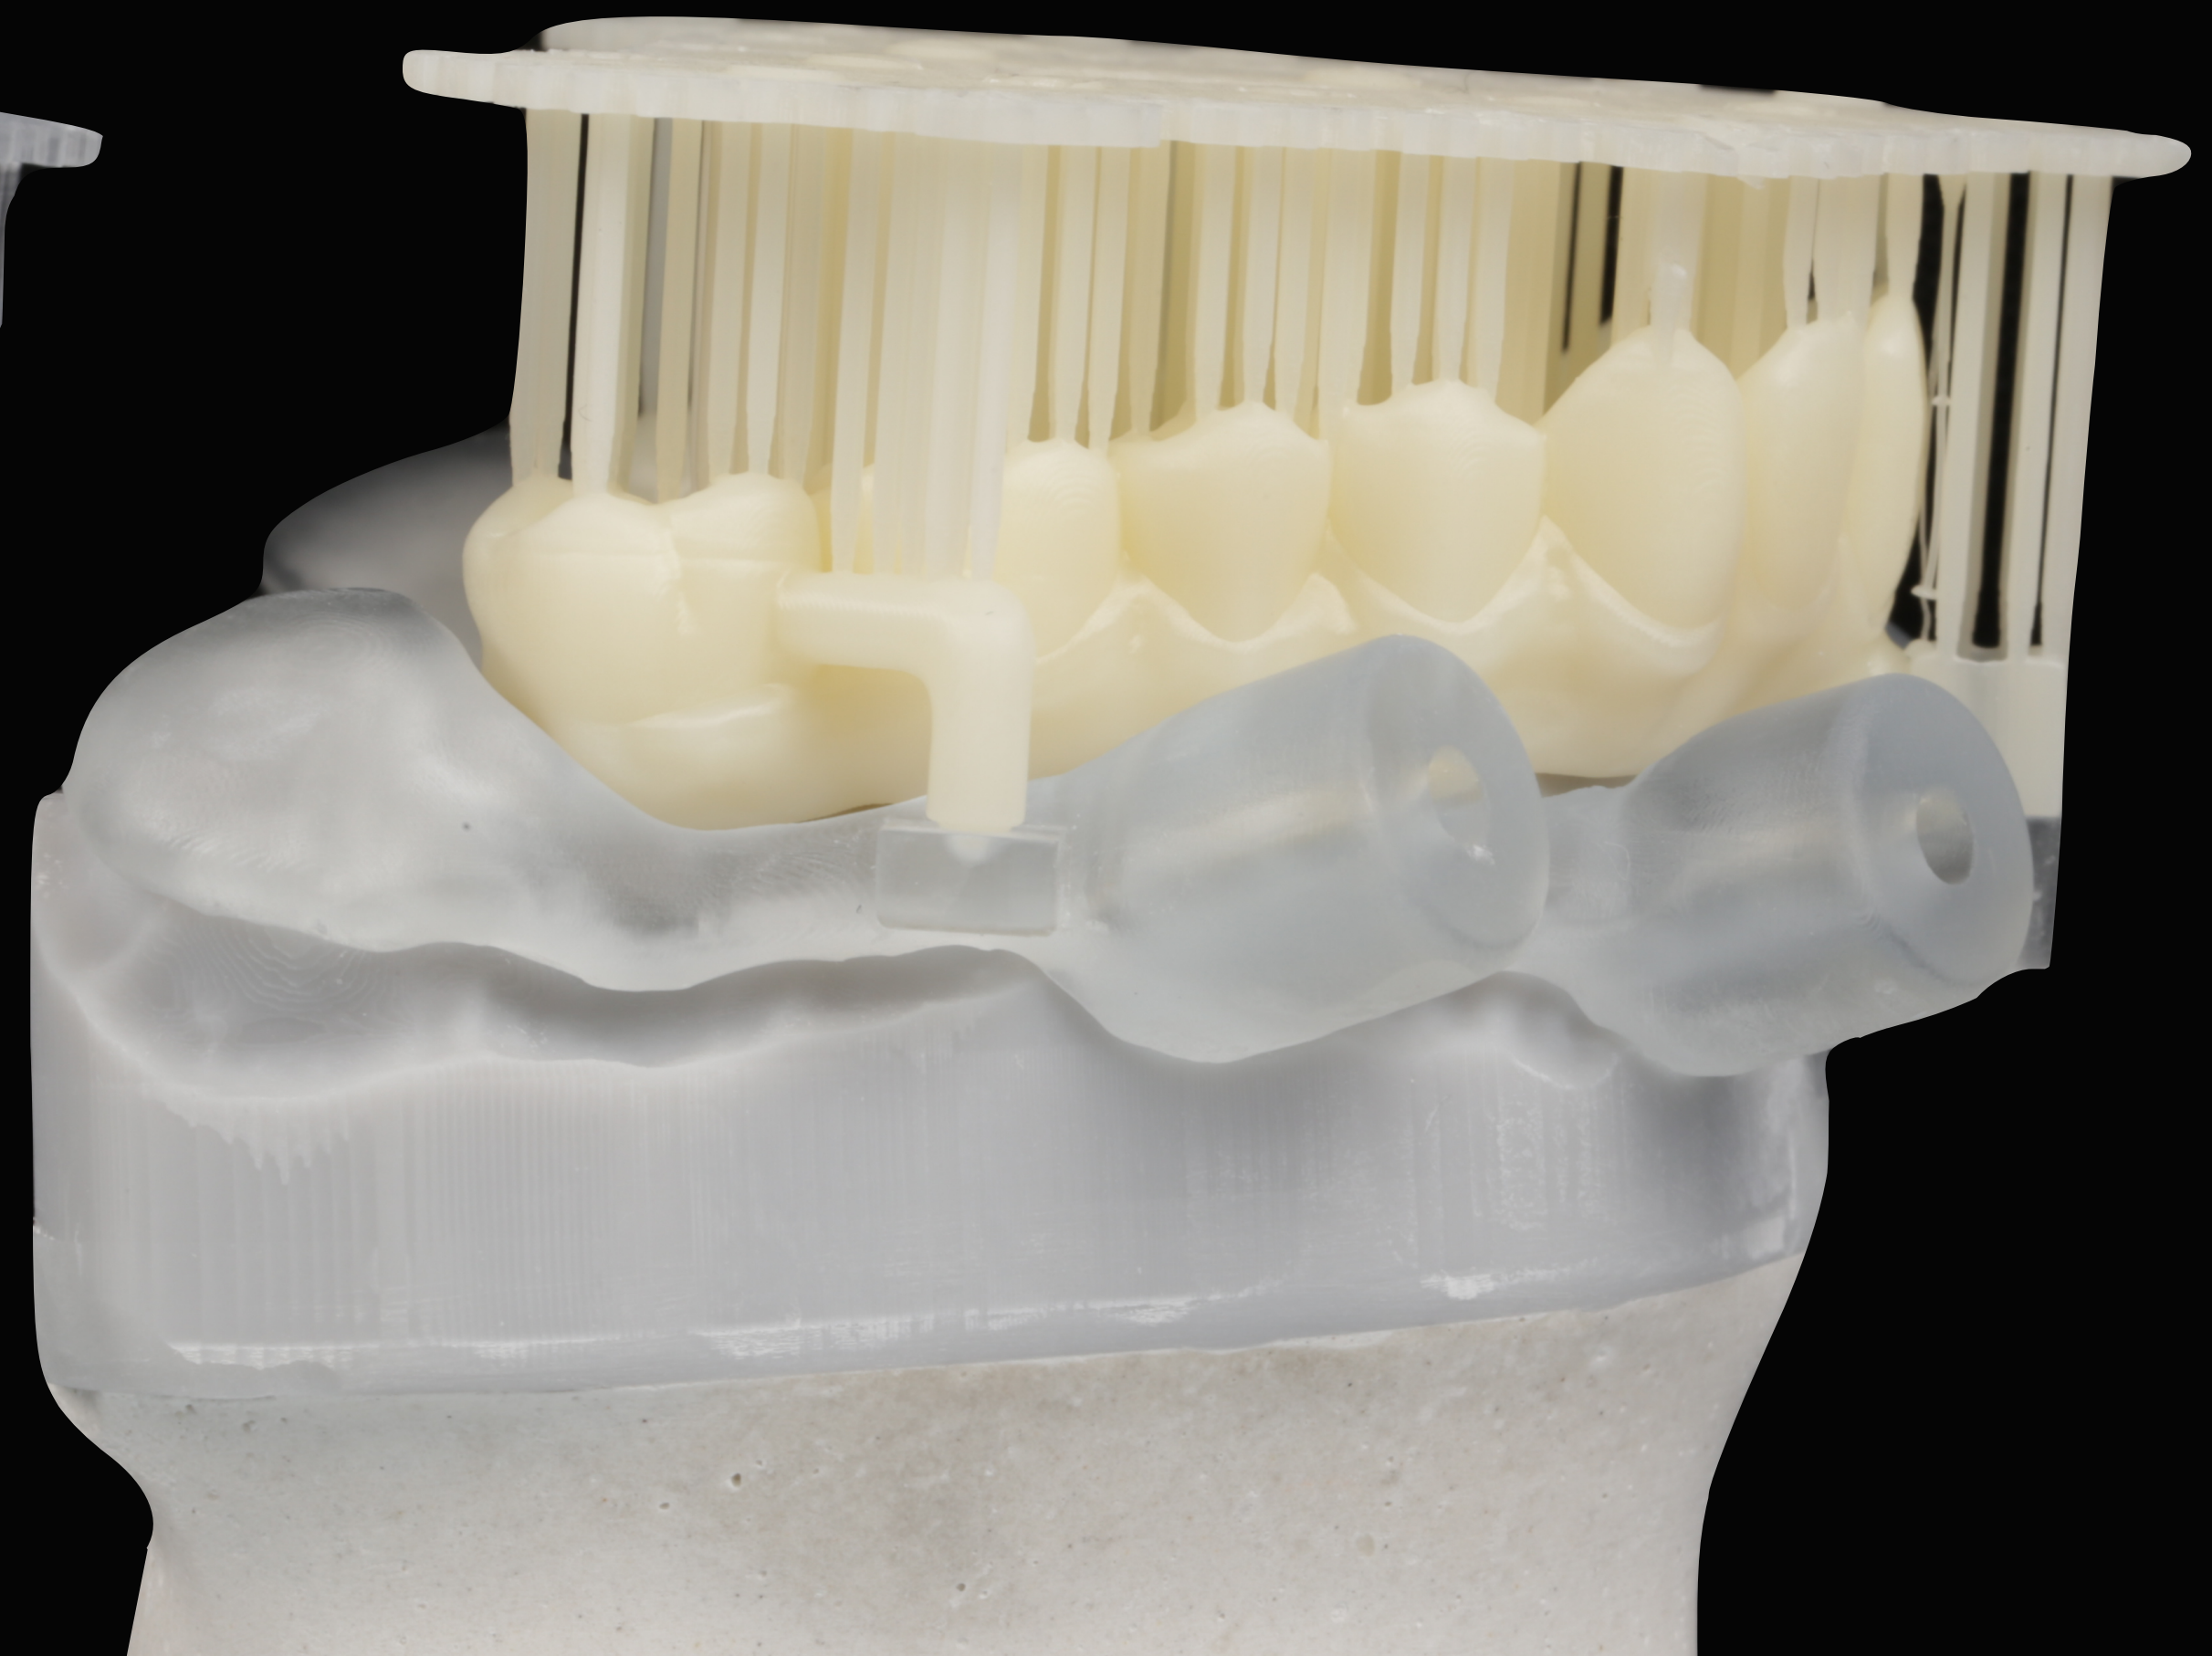

DR. ALEJANDRO JAMES OROZCO


ARTMES CONCEPT
FULL SET




BASE GUIDE



IMPLANT GUIDE

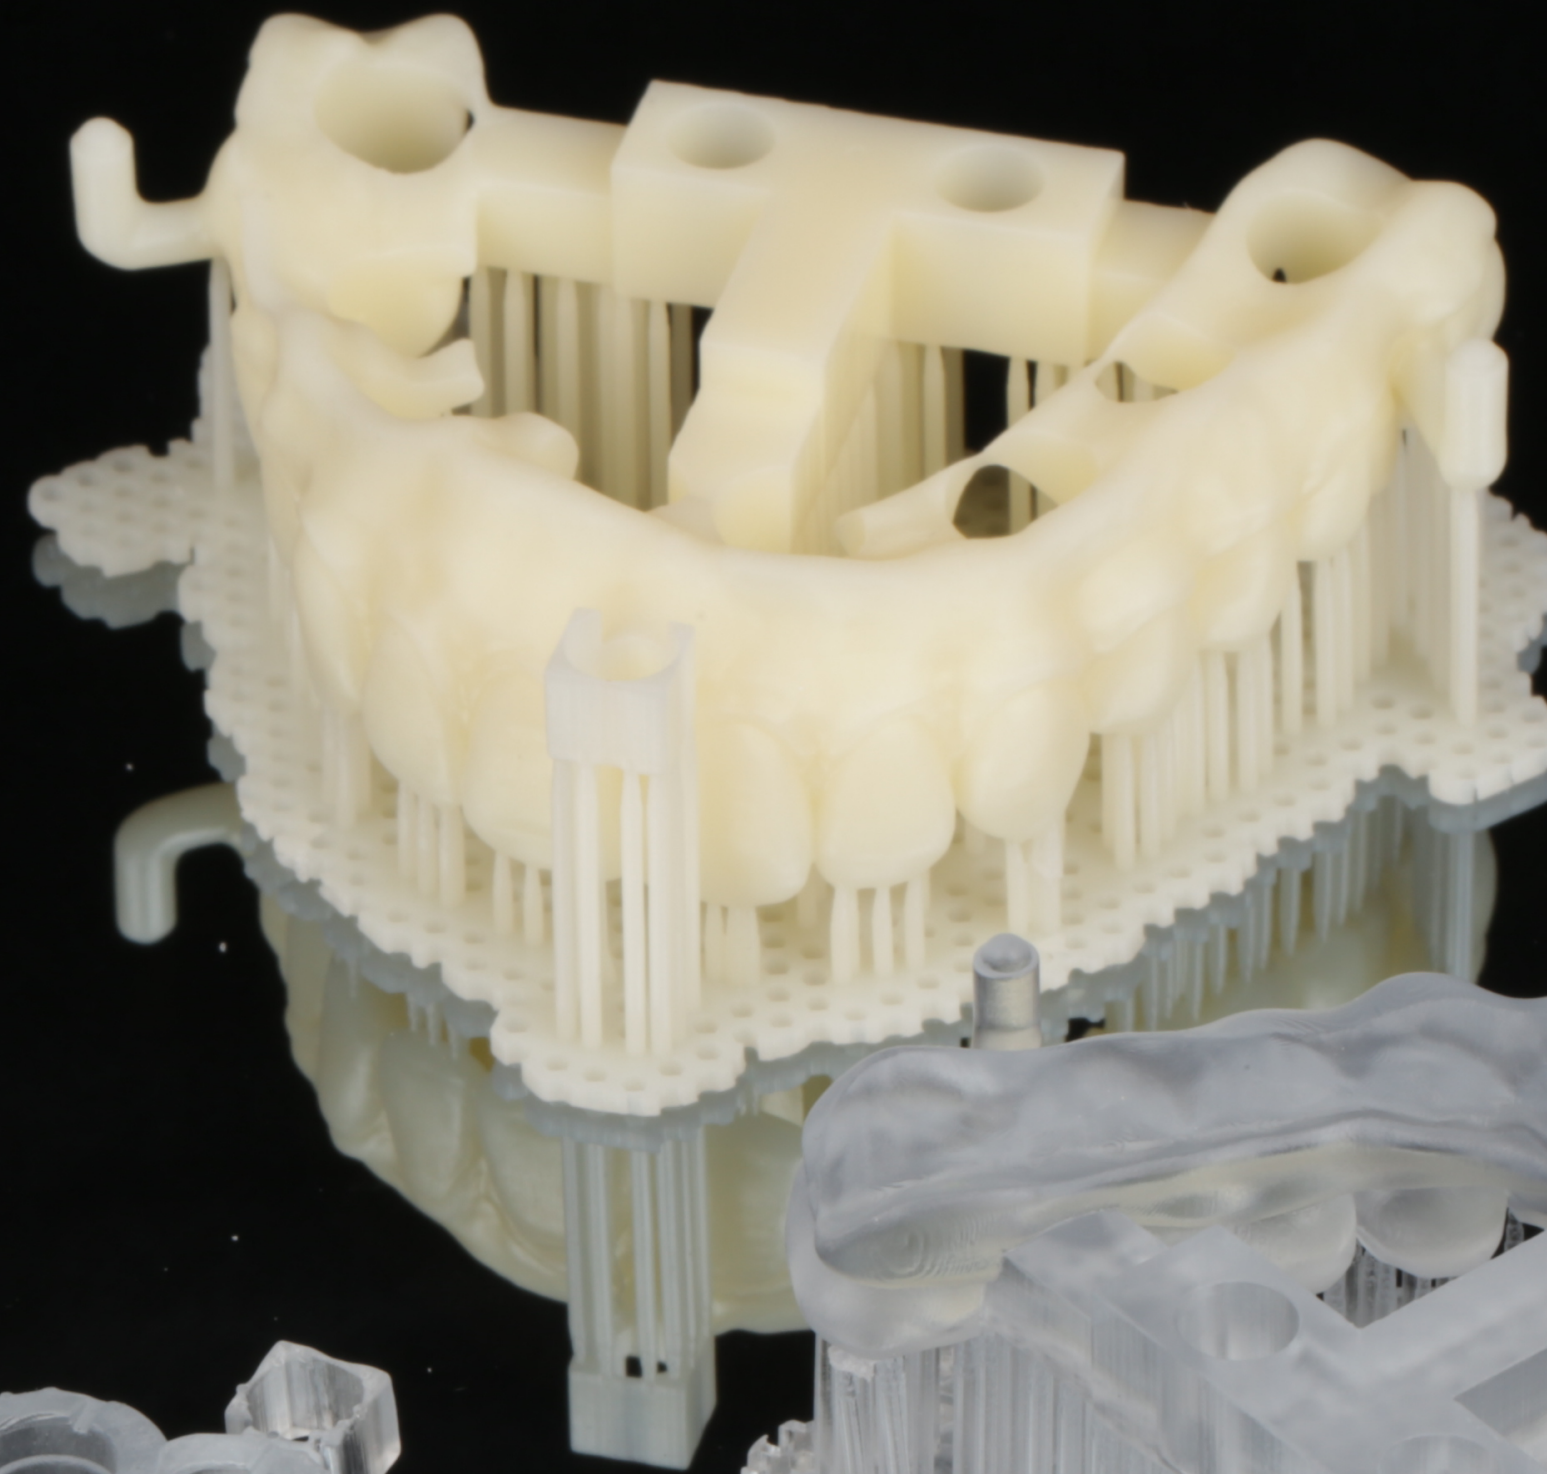

PROVISIONALS

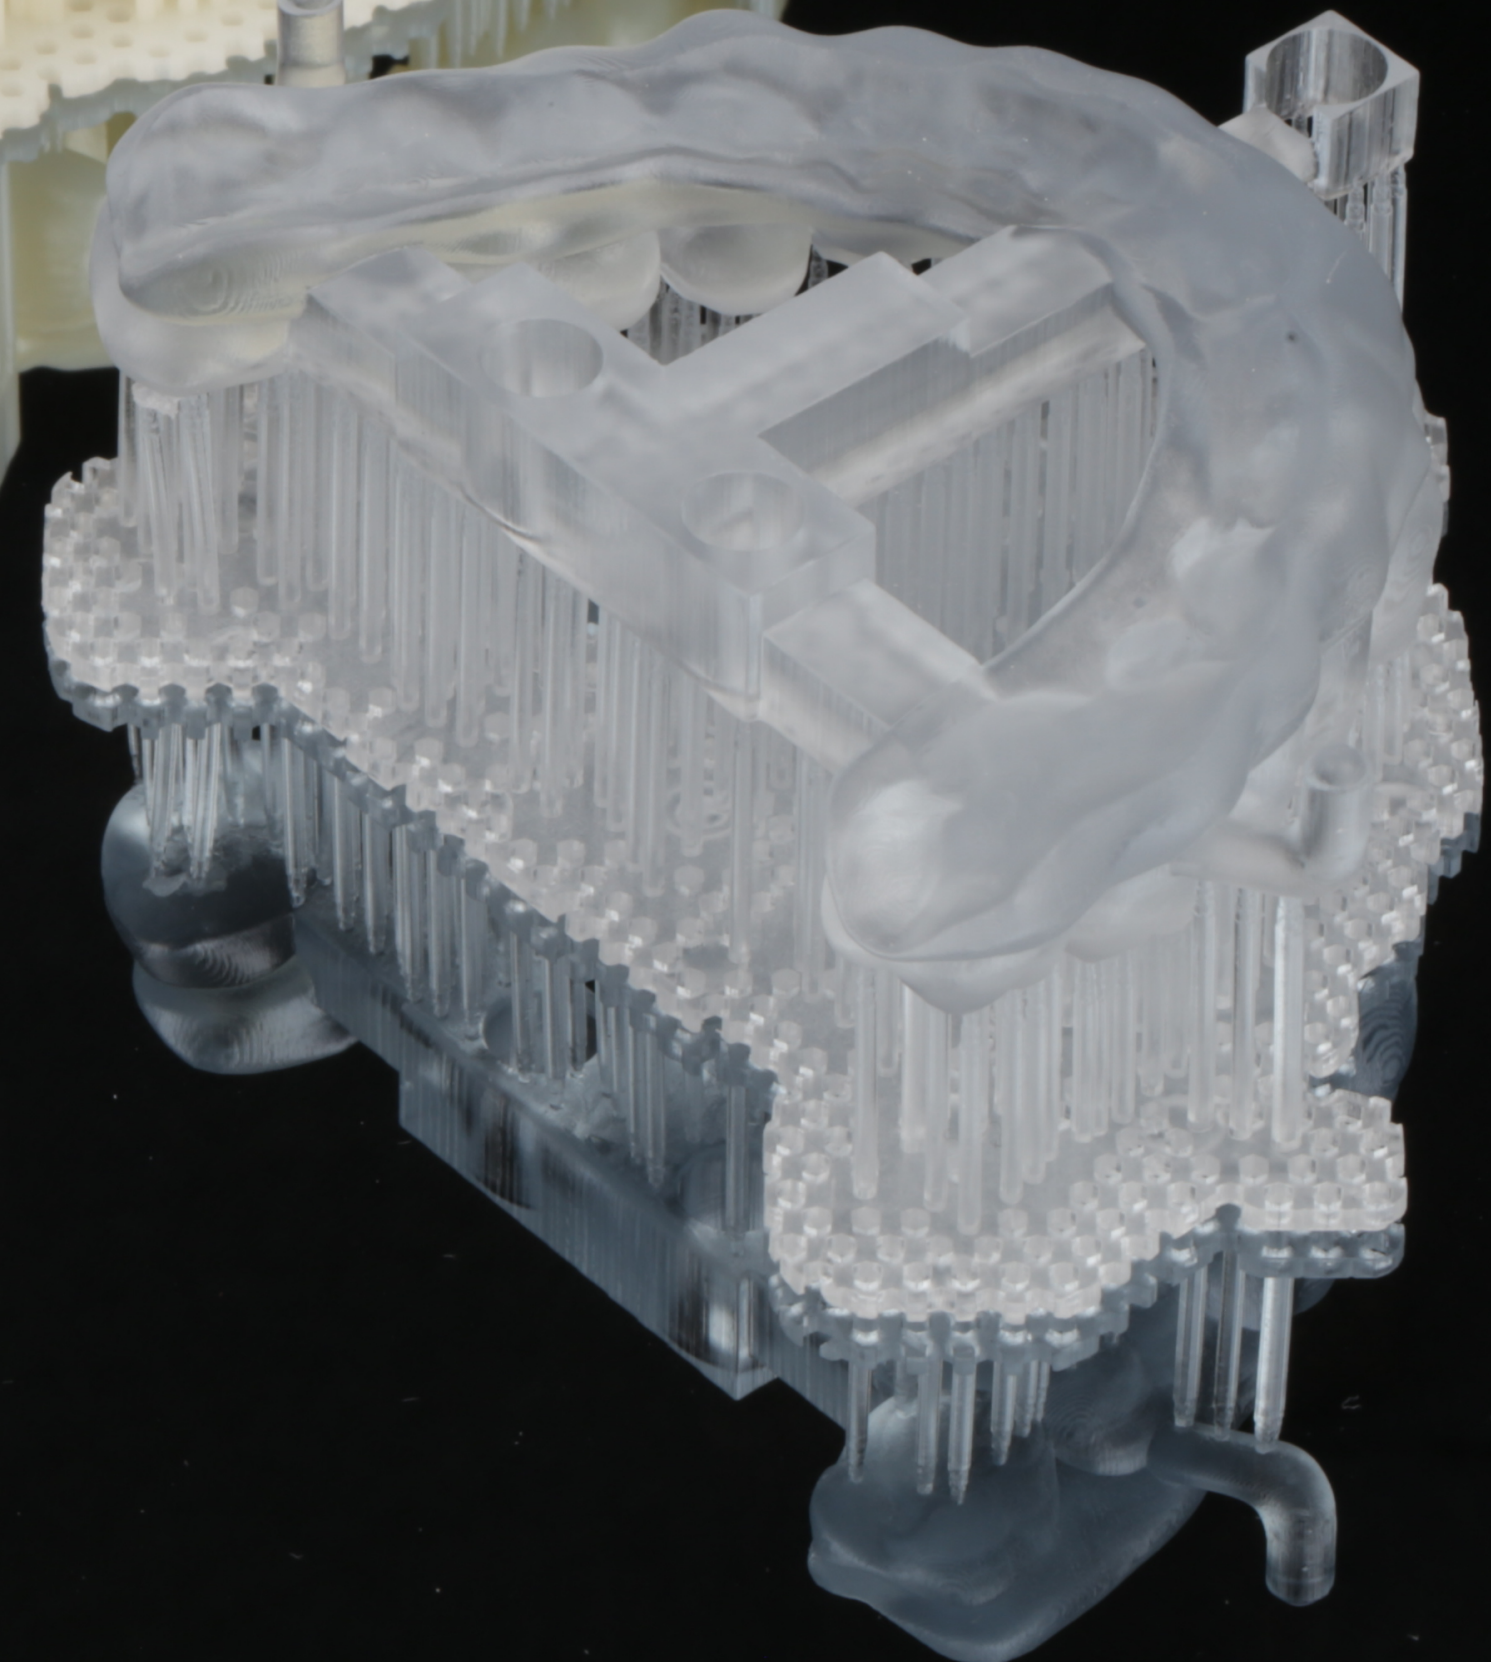

TRY-IN


DR. ALEJANDRO JAMES OROZCO



PICK-UP SITE PREPARATION
READY FOR 8 IMPLANTS




DR. ALEJANDRO JAMES OROZCO

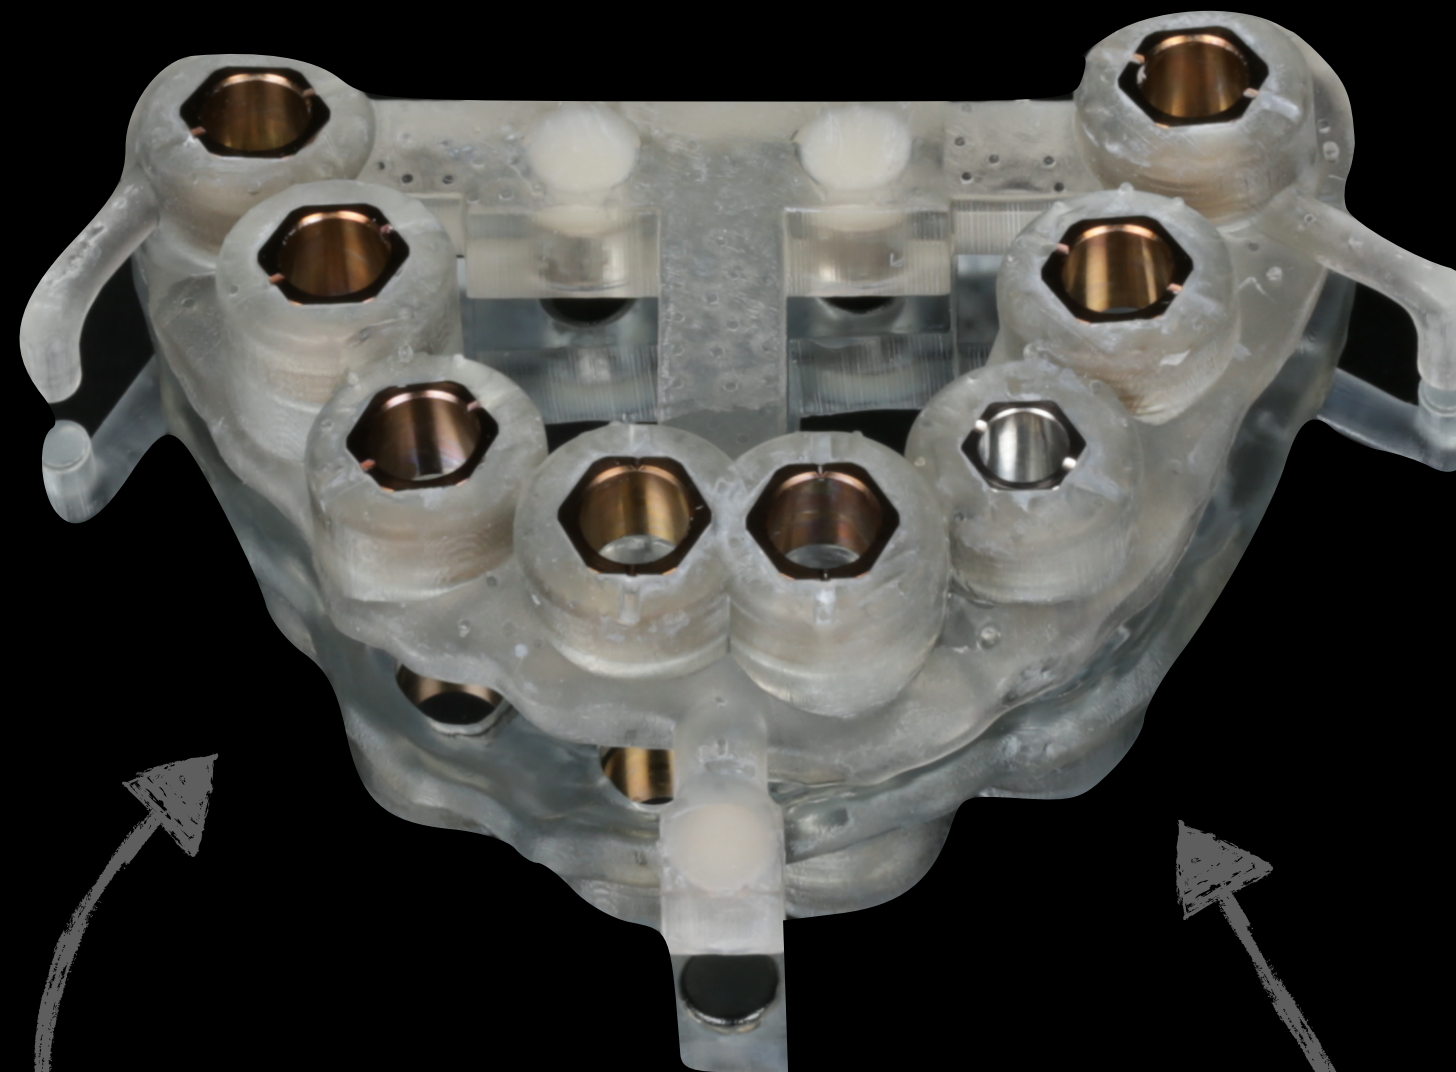



8 ANODIZED IMPLANT SLEEVES

DR. ALEJANDRO JAMES OROZCO

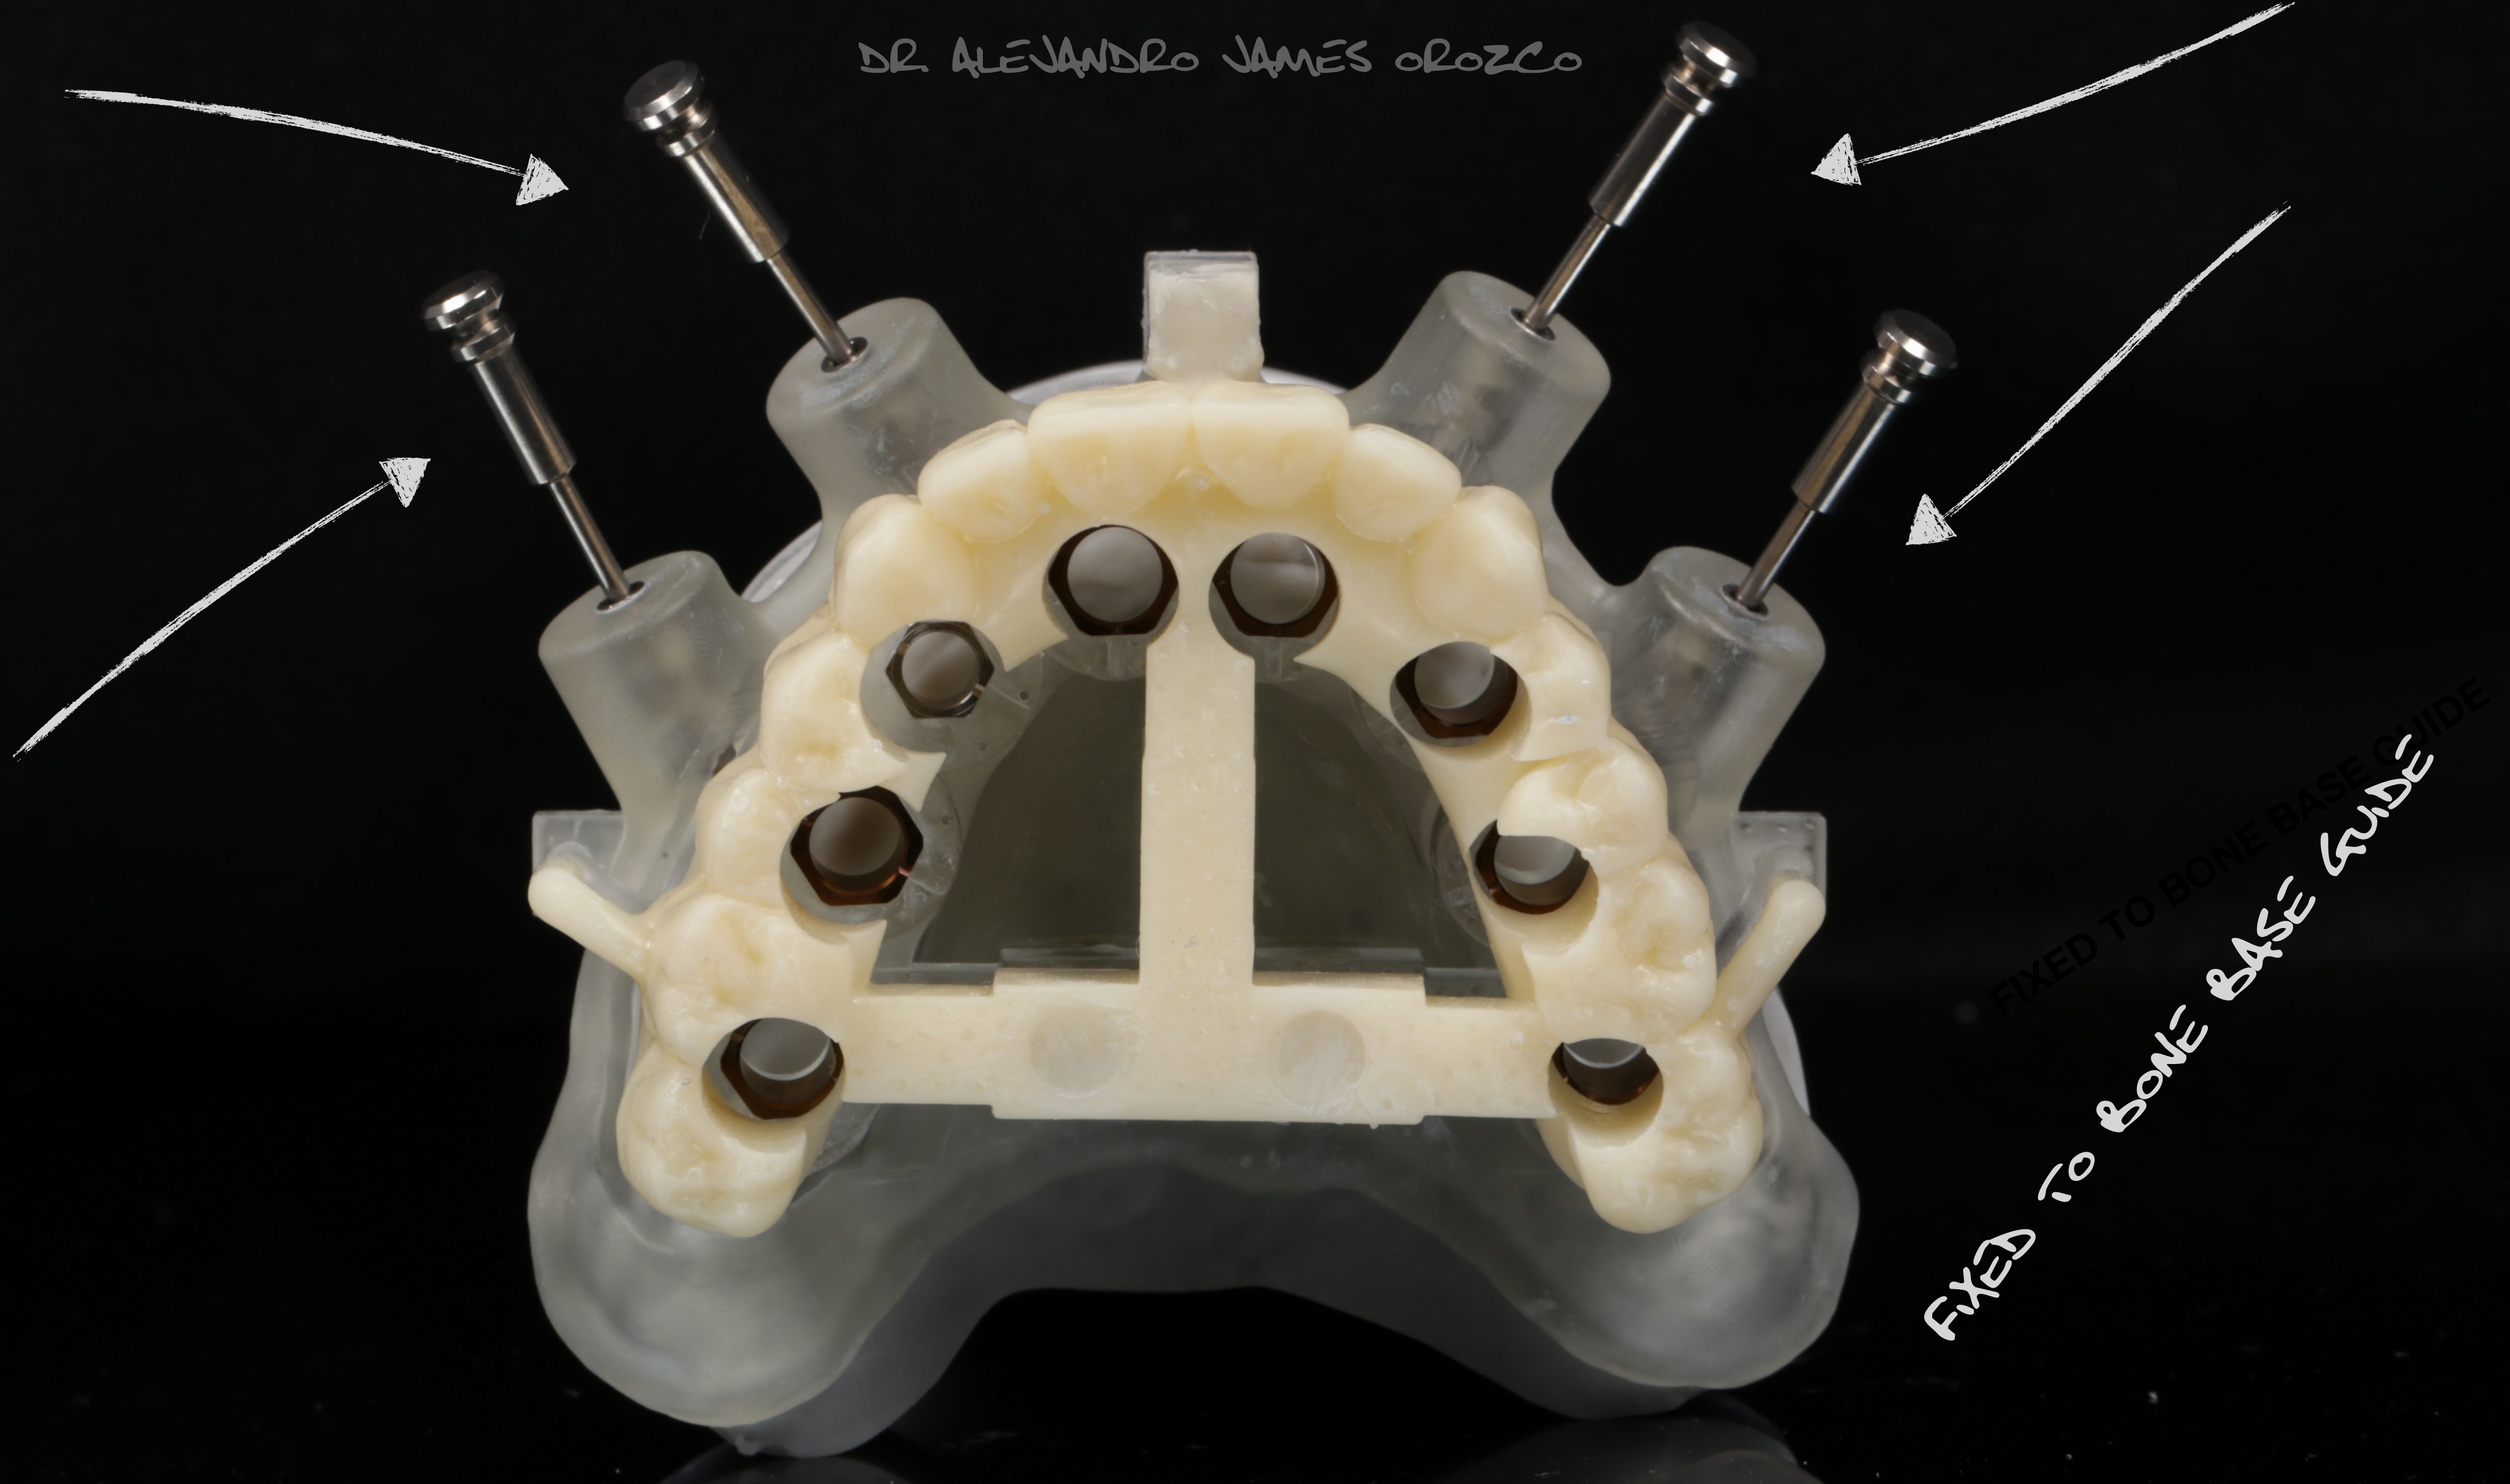

FIXED TO BONE BASE GUIDE
FIXED TO BONE BASE GUIDE

DR. ALEJANDRO JAMES OROZCO

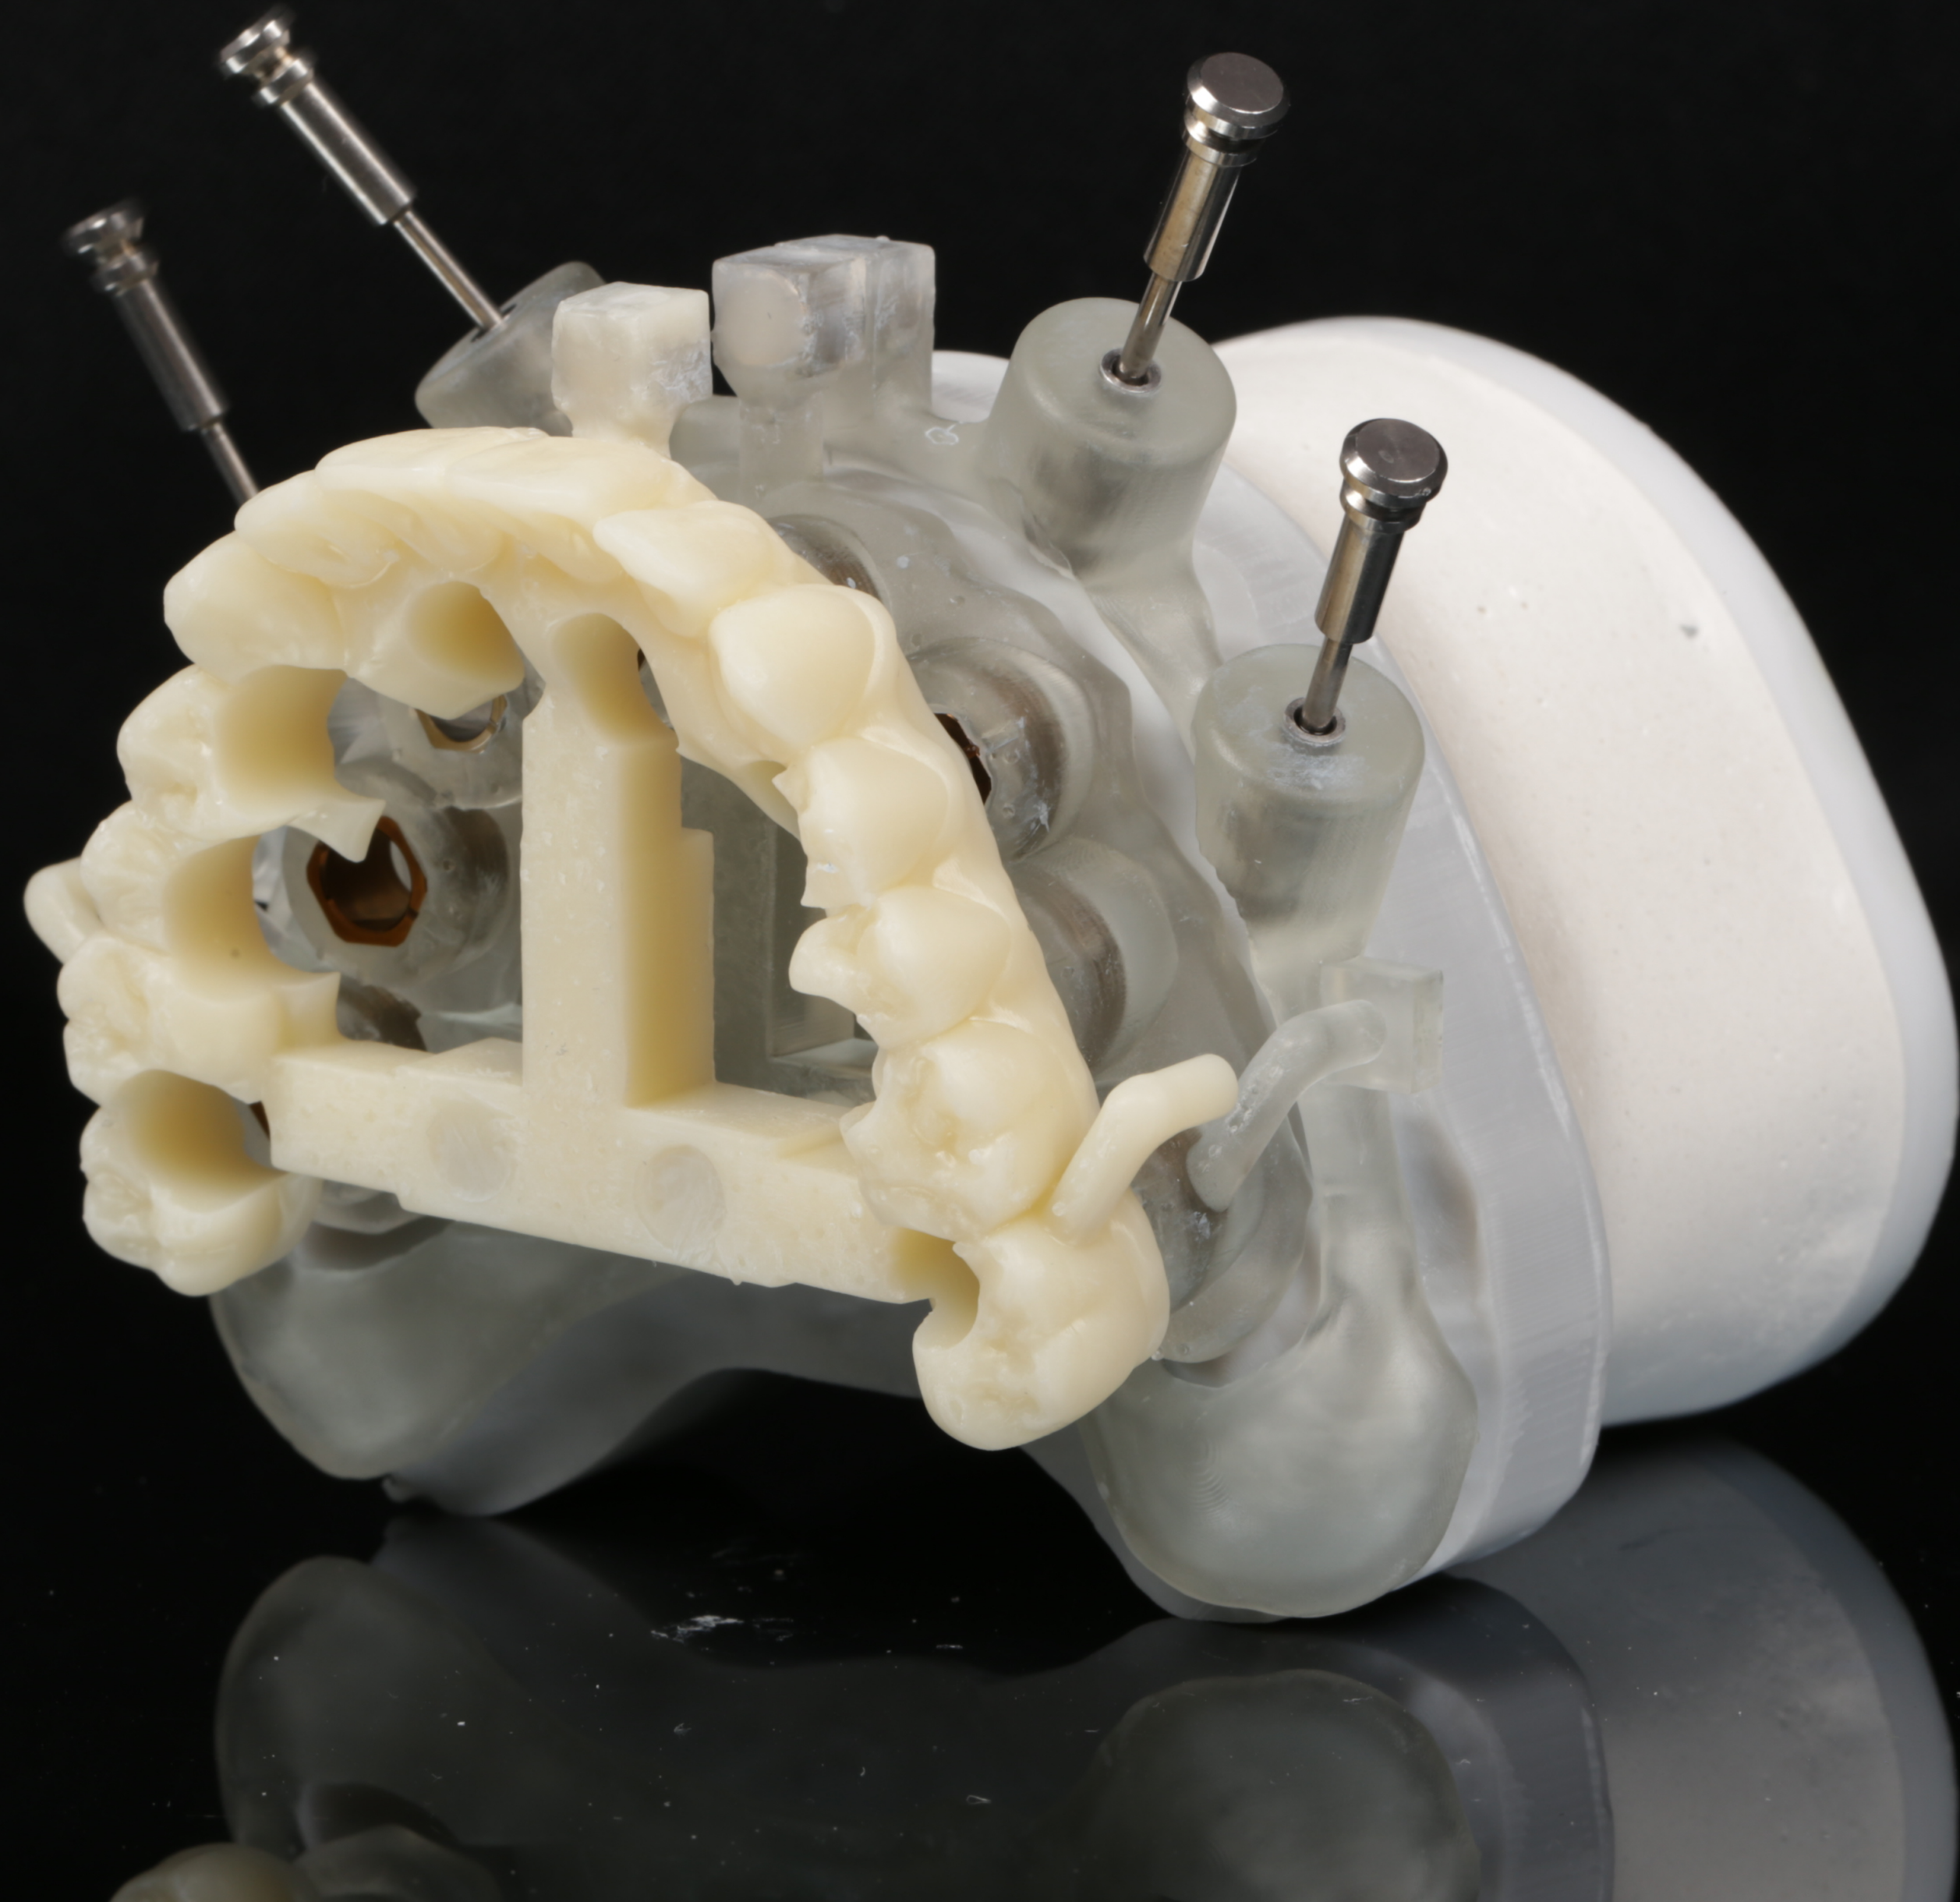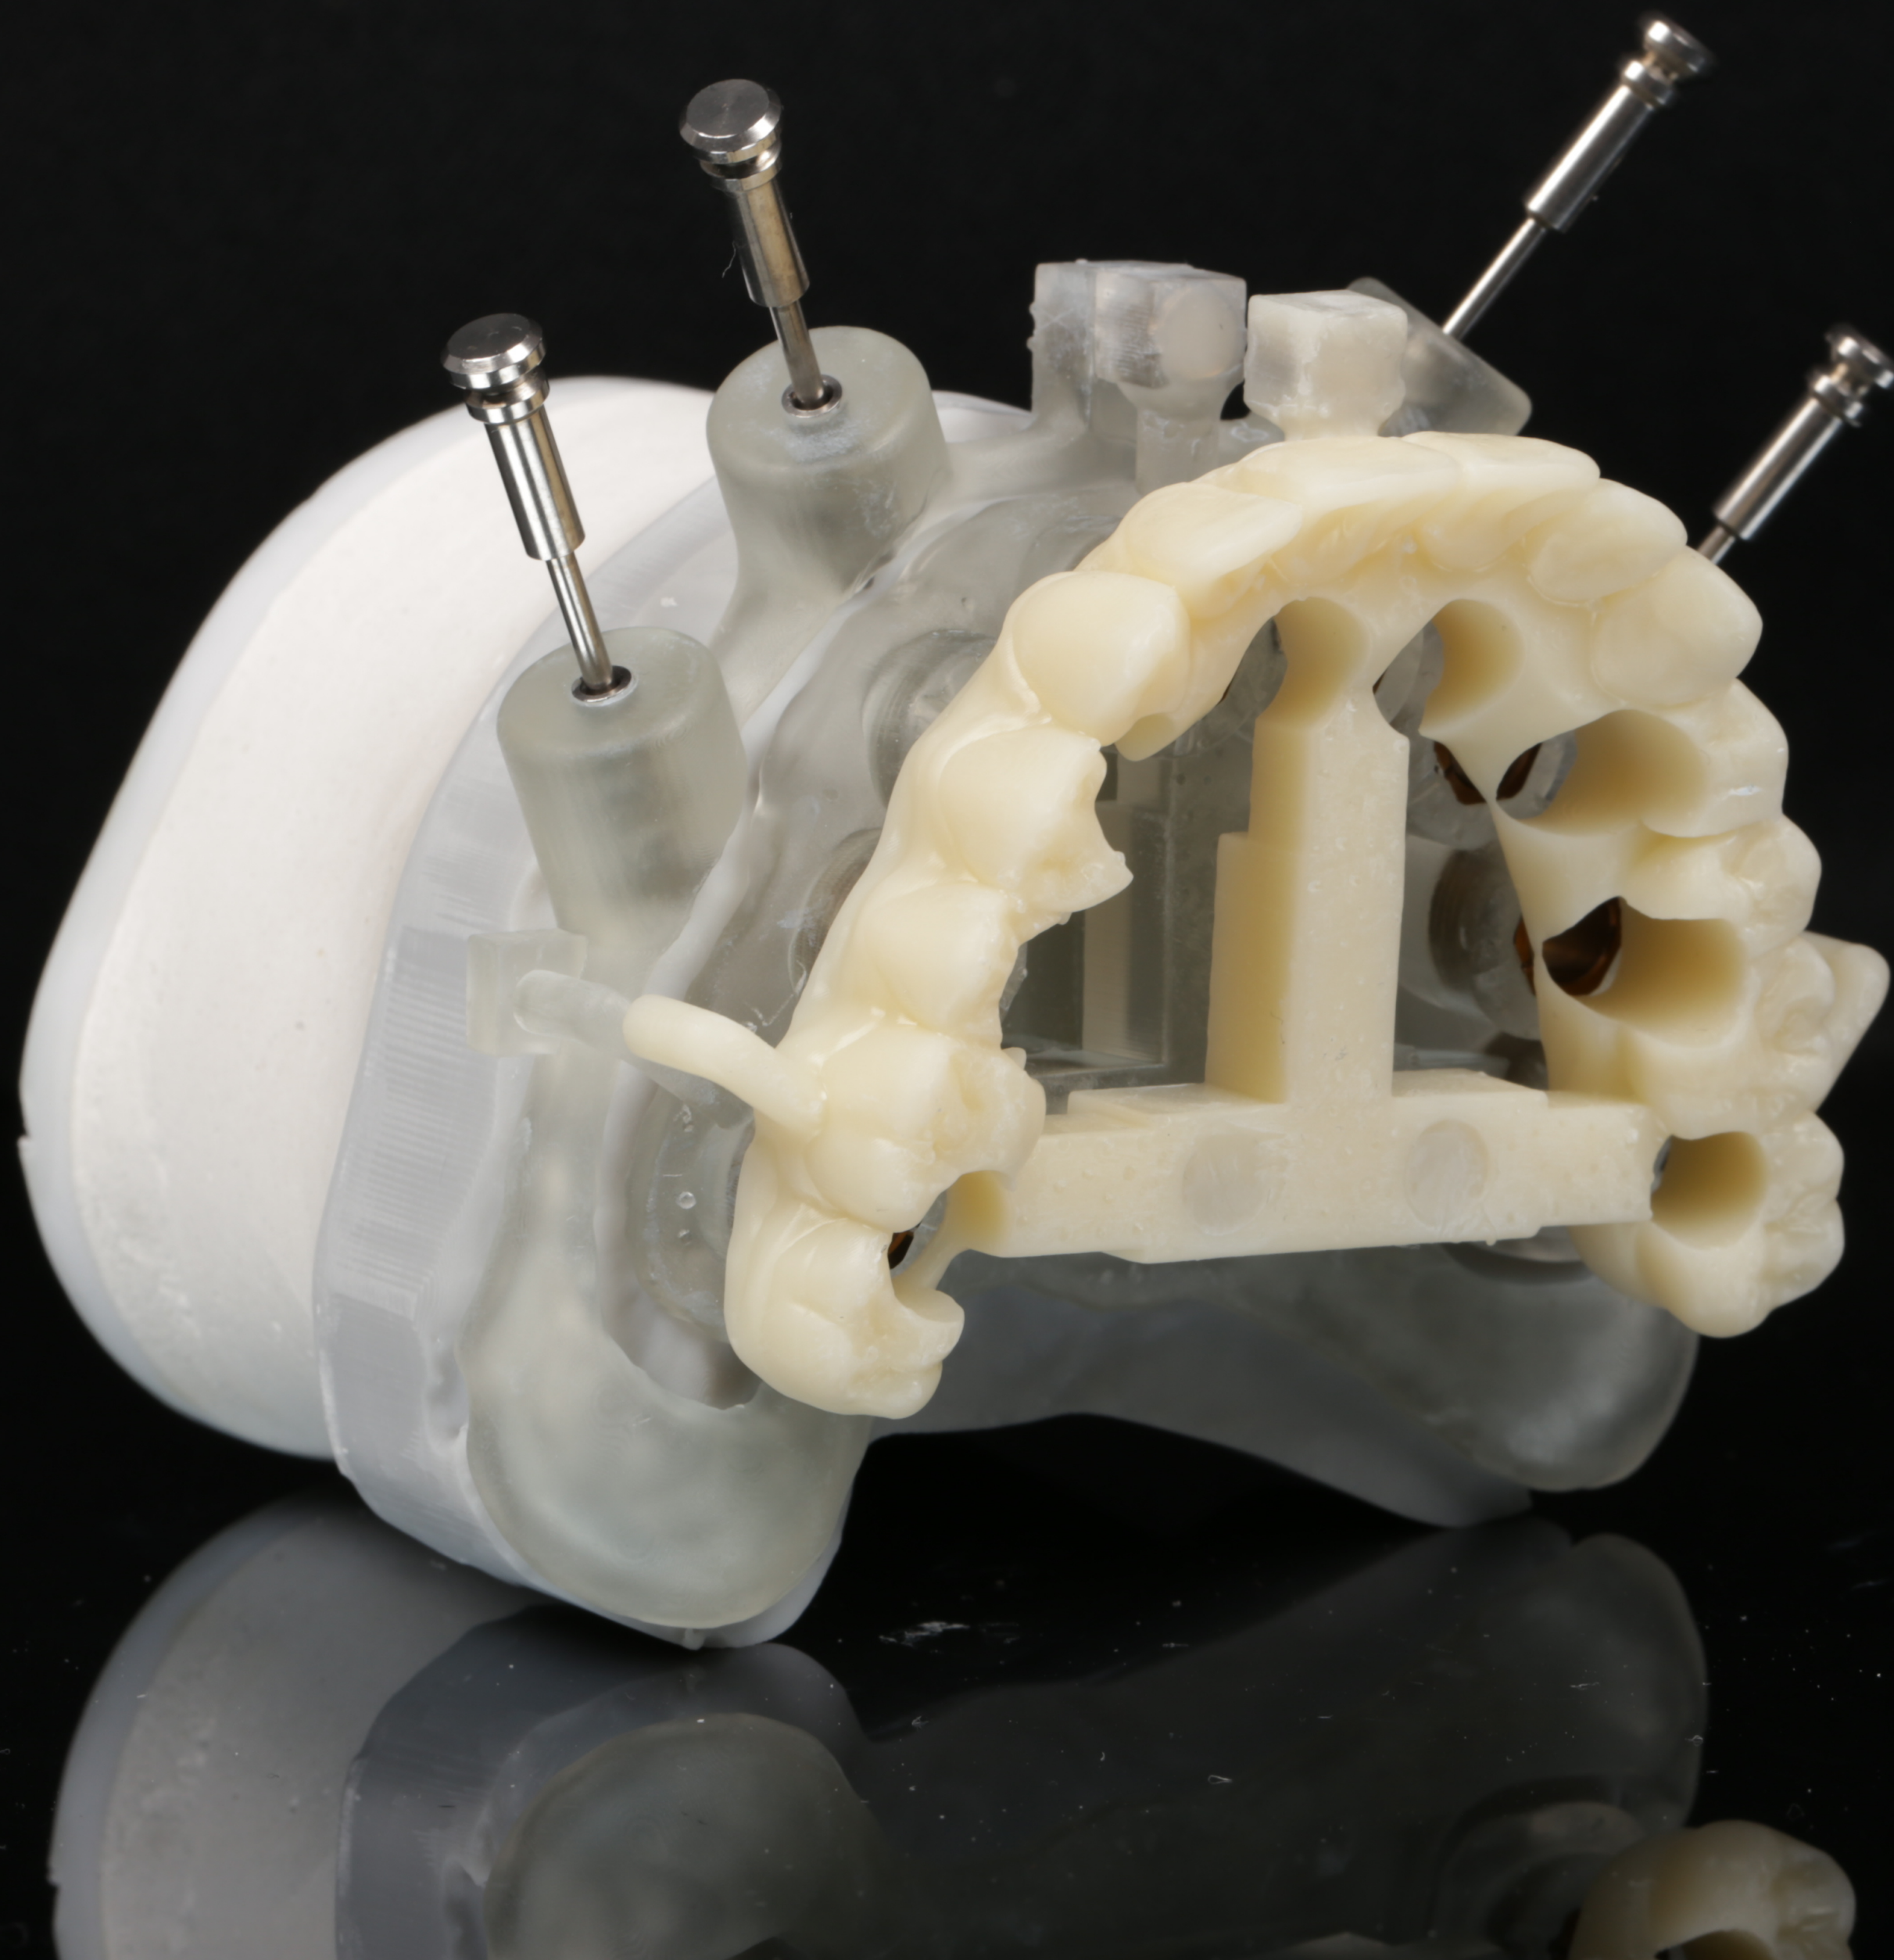

DGS
(DIGITAL GUIDANCE SLEEVE)








DR. ALEJANDRO JAMES OROZCO

TAPERED / ACTIVE APEX

K-LEAN SURFACE

PLATFORM SWITCHING

ENHANCED STABILITY
Dynamic

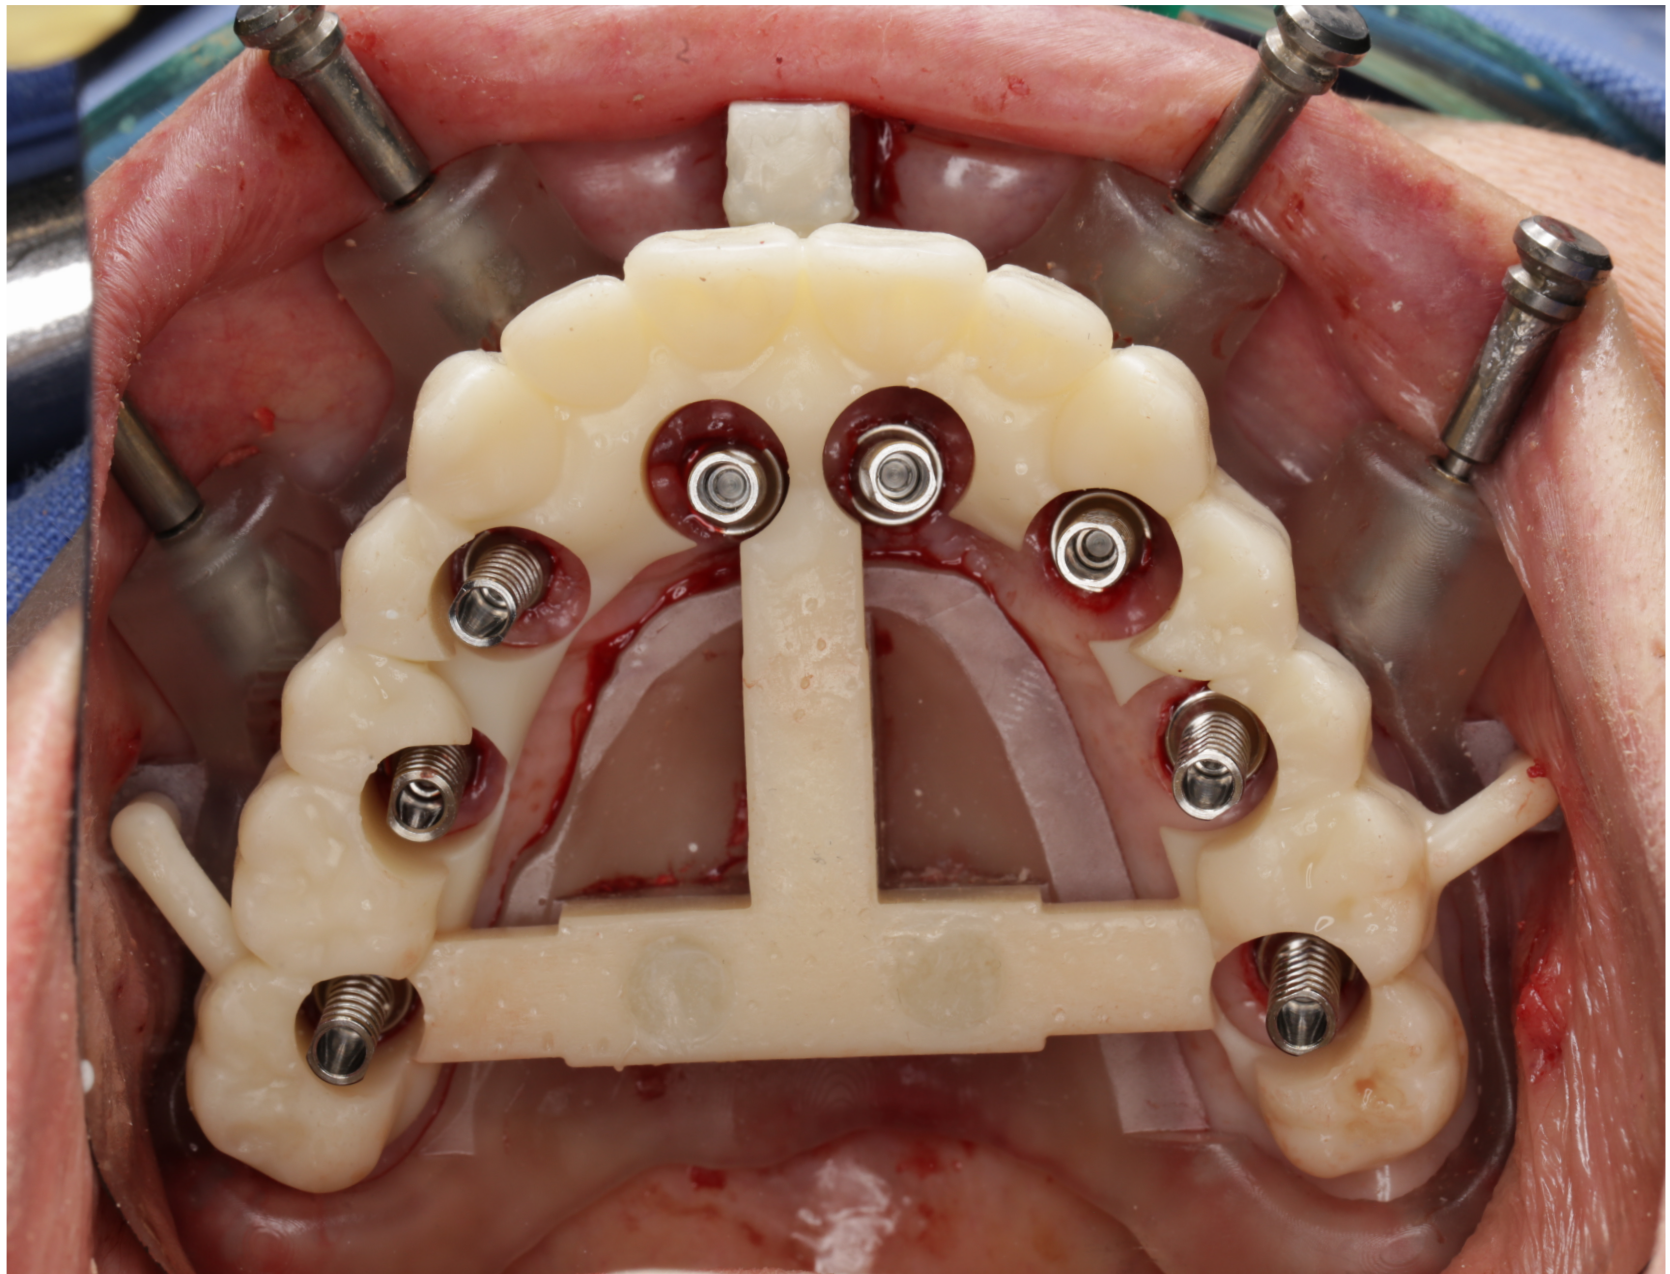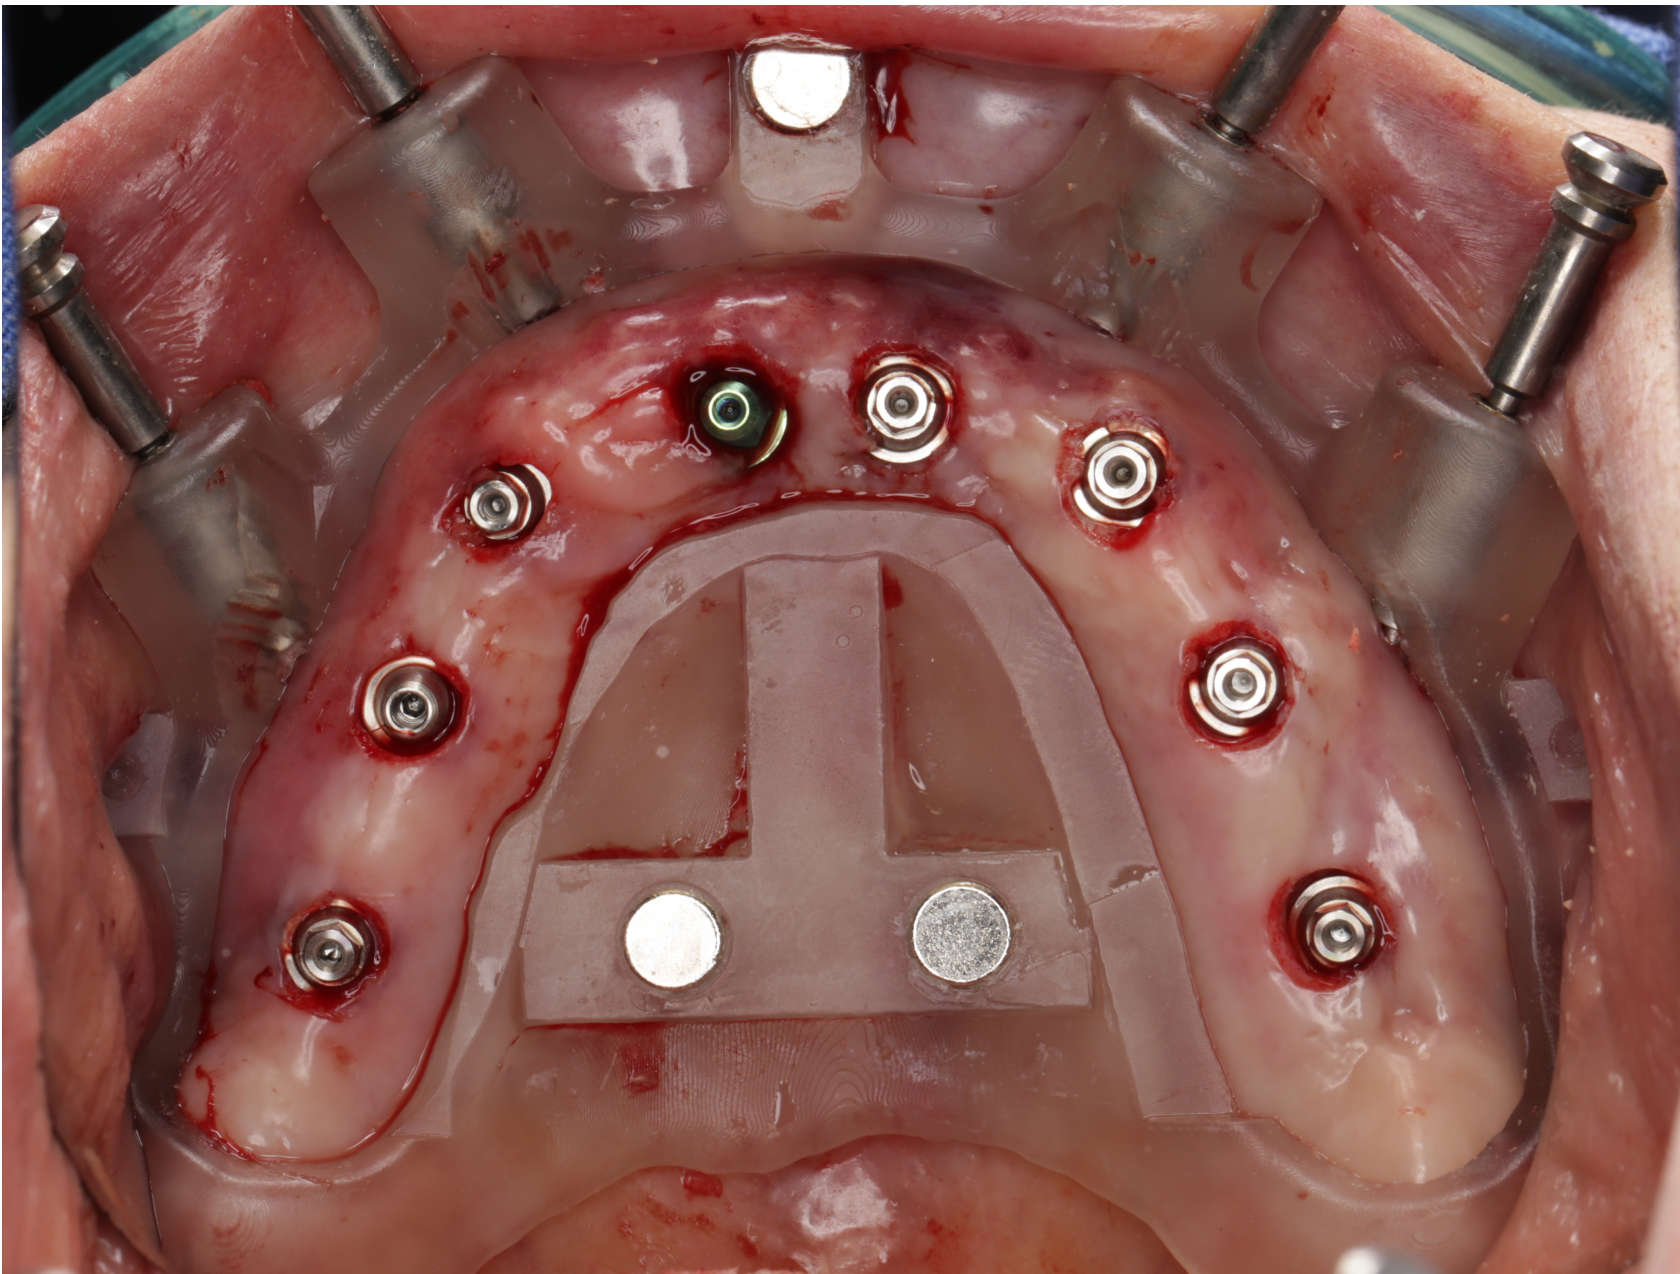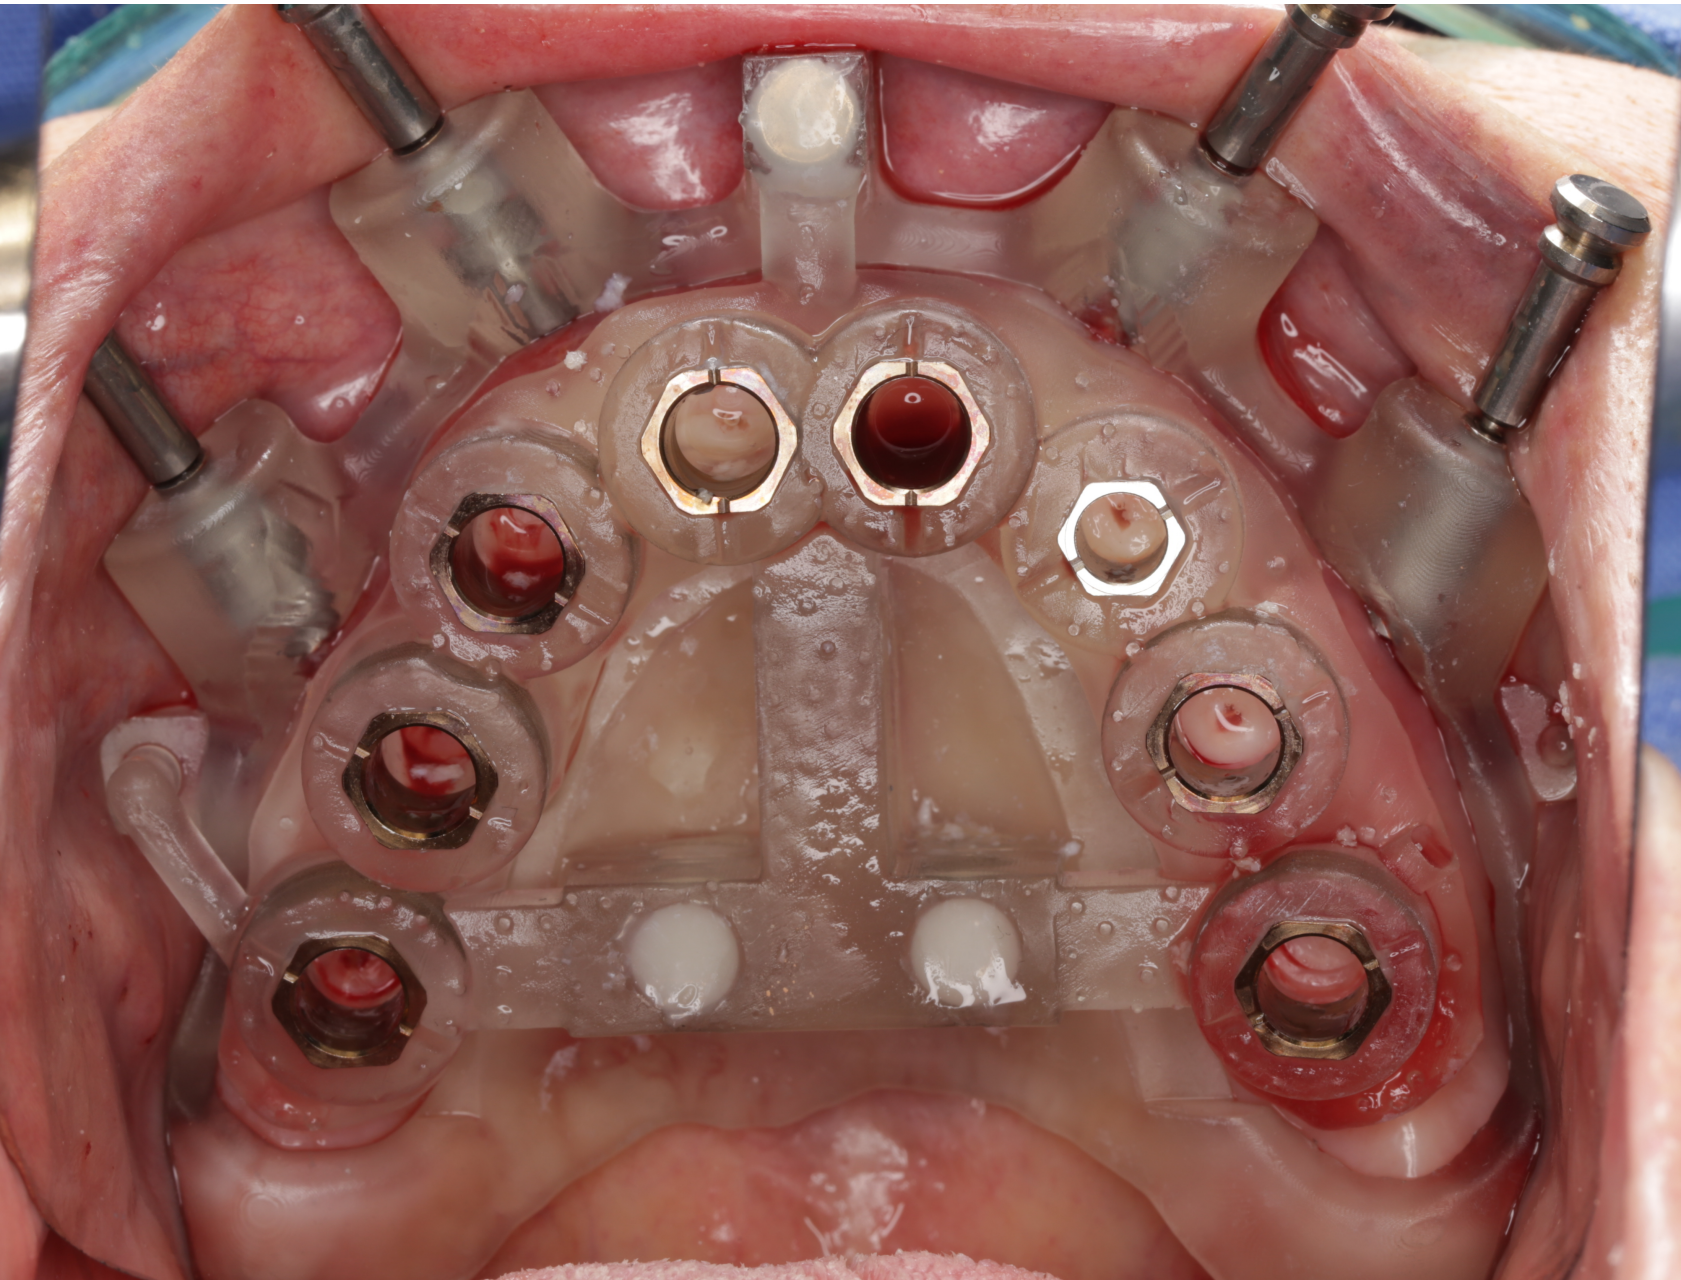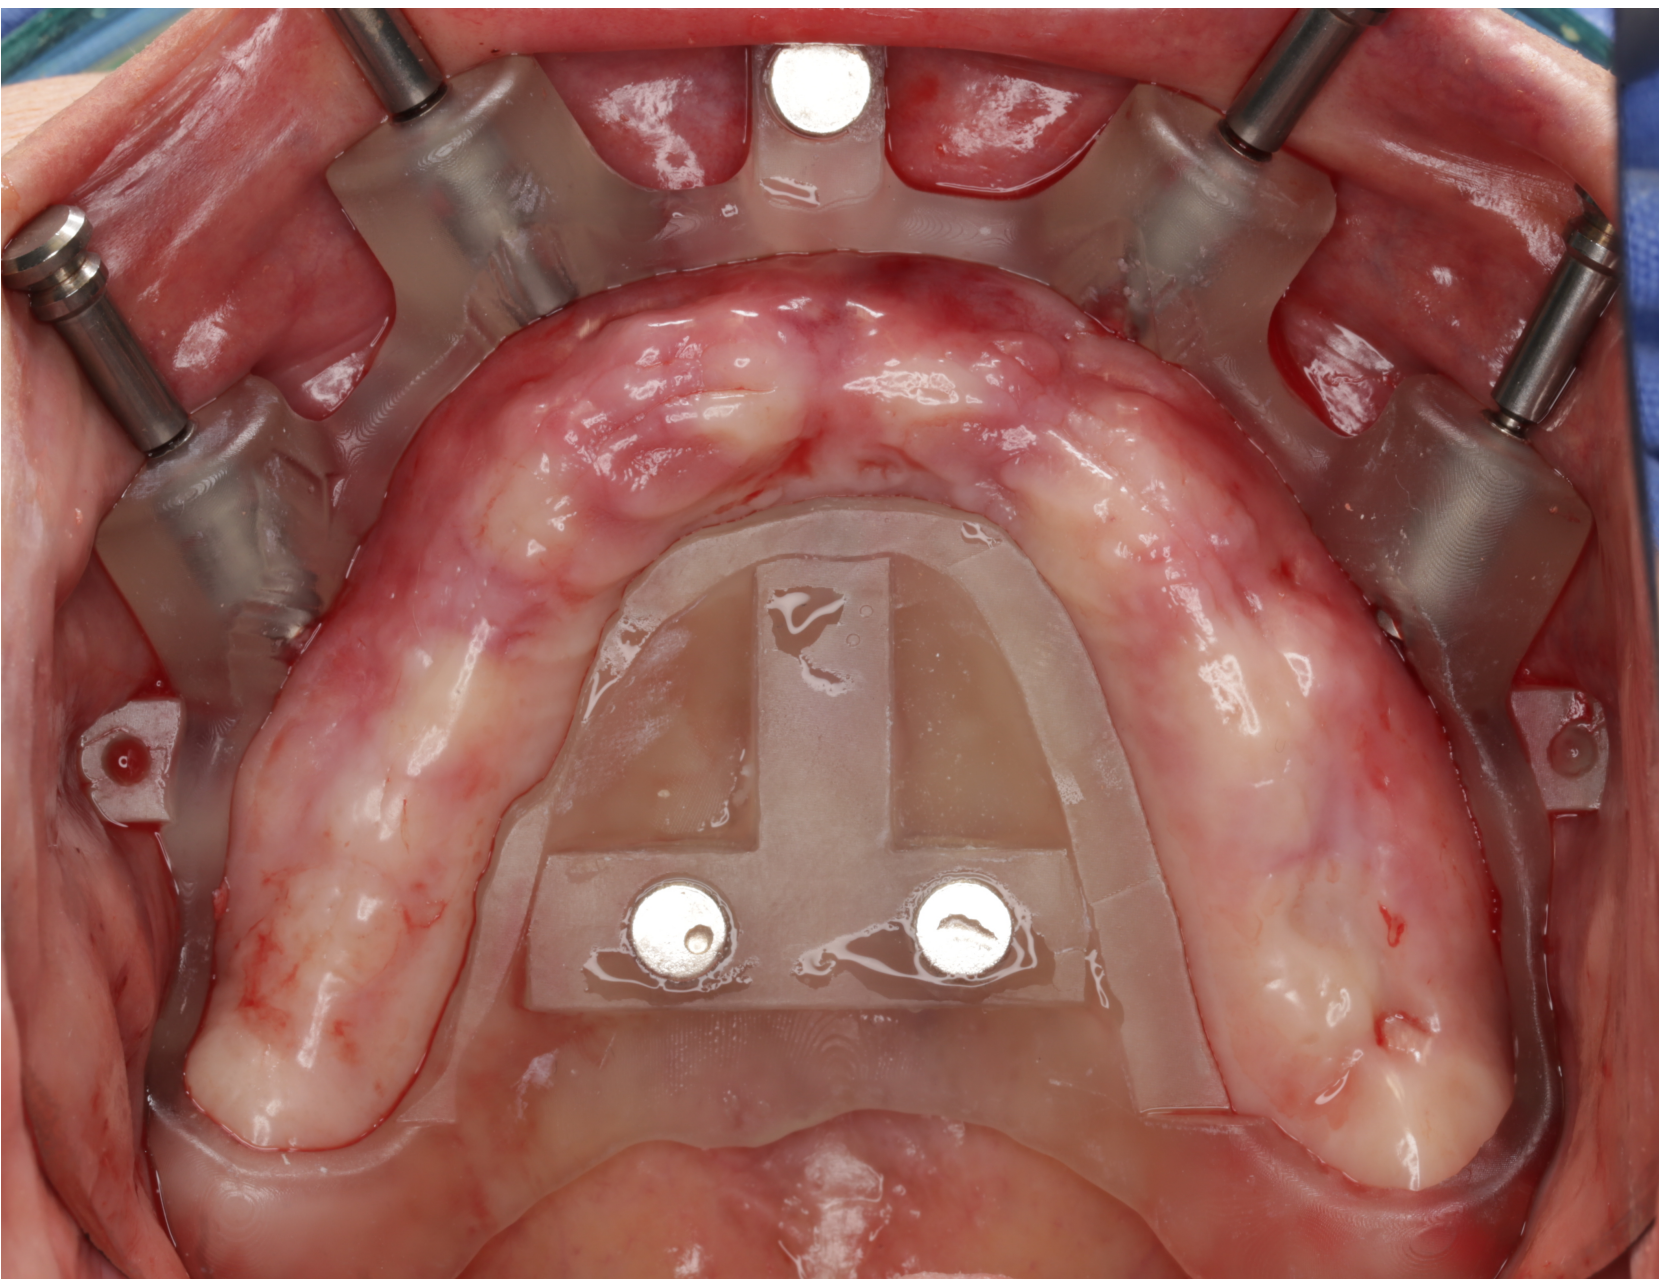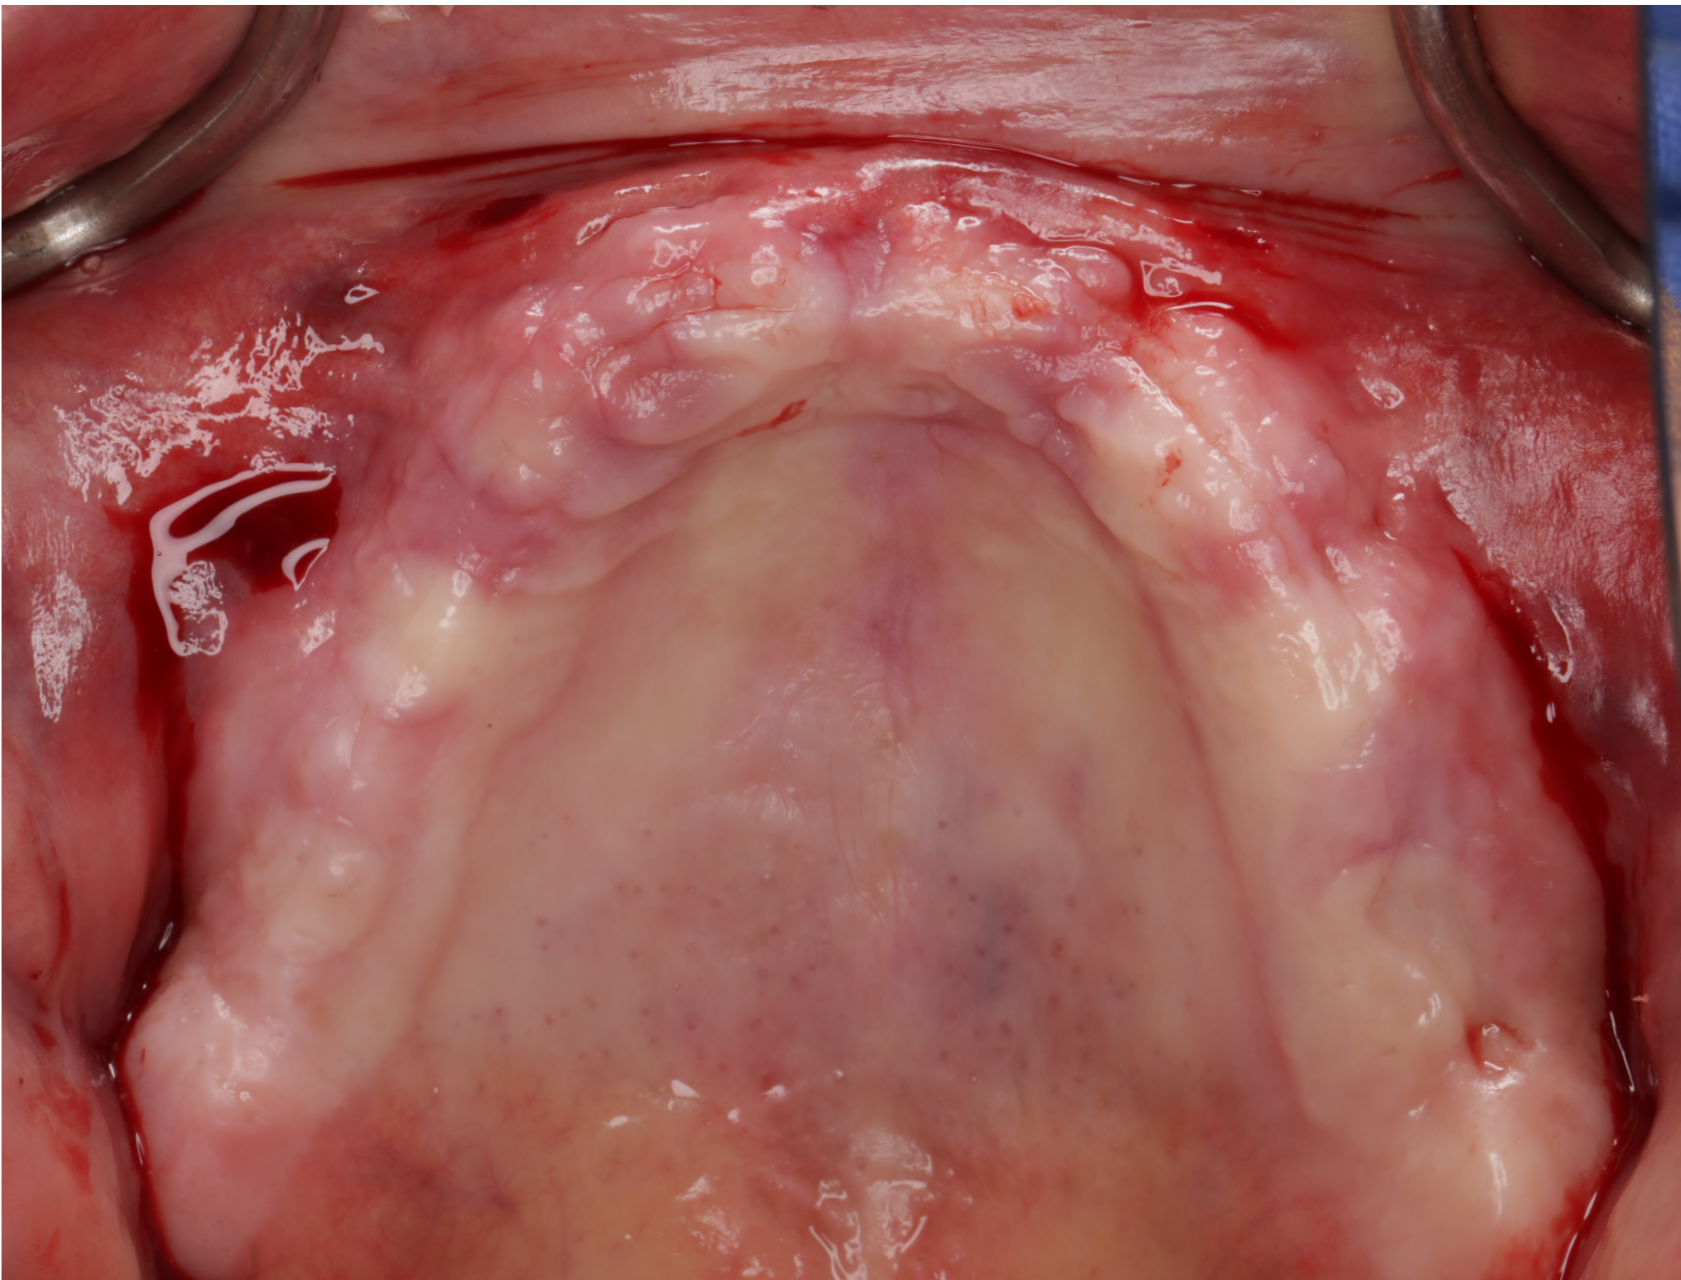

DR. ALEJANDRO JAMES OROZCO

GLAZE
AND
PICKUP
FOR
PRINTED
PROVISIONAL





DR. ALEJANDRO JAMES OROZCO

FLOWABLE GINGIVA



DR. ALEJANDRO JAMES OROZCO

